


=====

Acq. Operator	: System	Seq. Line	: 2
Acq. Instrument	: LC1260	Location	: Vial 4
Injection Date	: 2/18/2016 11:03:25 PM	Inj	: 1
		Inj Volume	: 0 µl
Different Inj Volume from Sequence !		Actual Inj Volume	: 2 µl
Acq. Method	: E:\DATA\Data\20160218\20130913-01 2016-02-18 22-37-00\30-90 AD 15MIN.M		
Last changed	: 2/18/2016 10:37:00 PM by System		
Analysis Method	: D:\PUBLIC\METHOD\30-90 6MIN.M		
Last changed	: 1/28/2016 11:00:39 AM		

=====

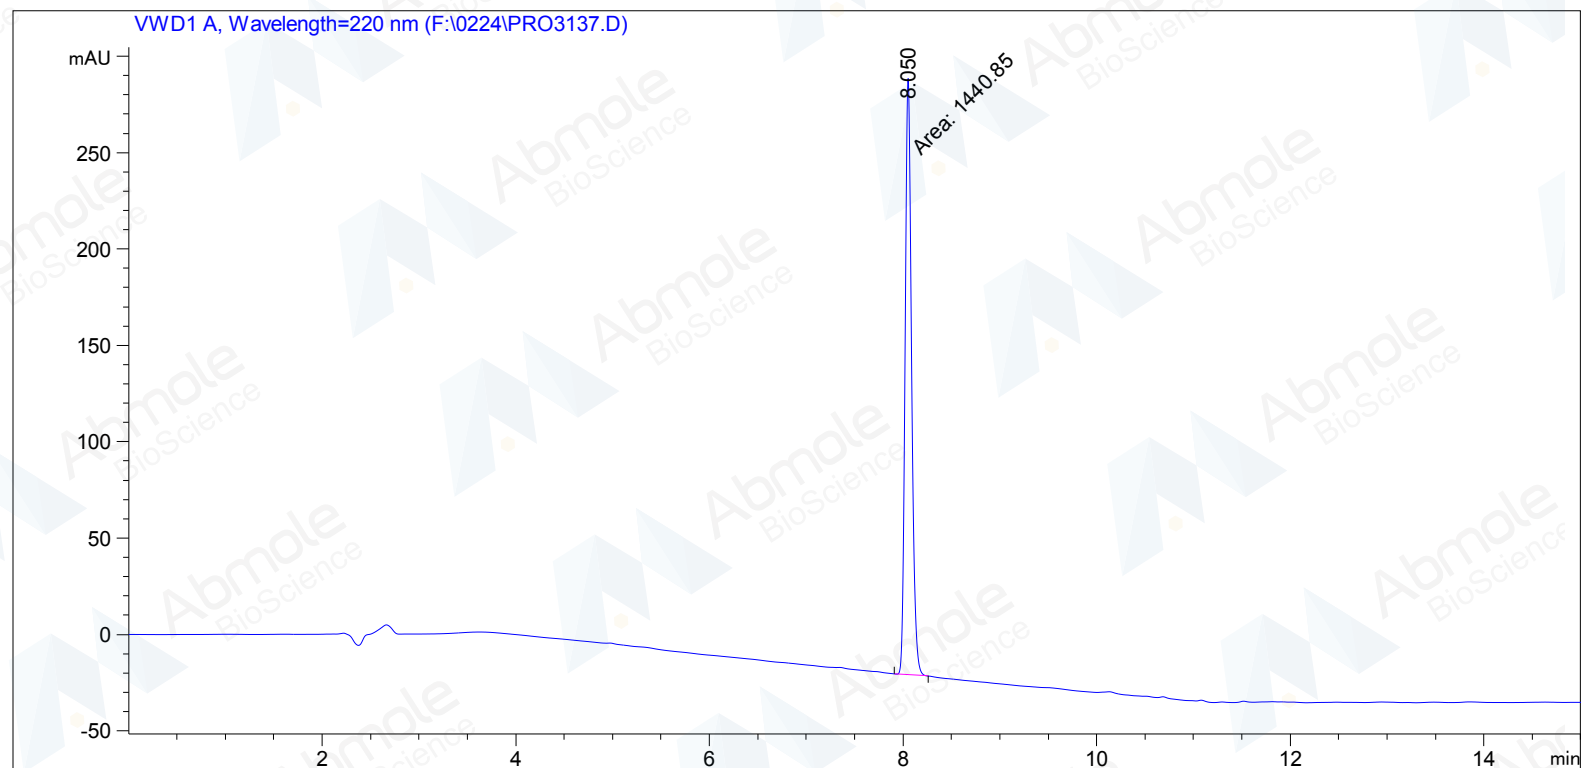

=====

Area Percent Report

=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=220 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.050	MM	0.0775	1440.84680	309.66772	100.0000

Totals : 1440.84680 309.66772

*** End of Report ***