
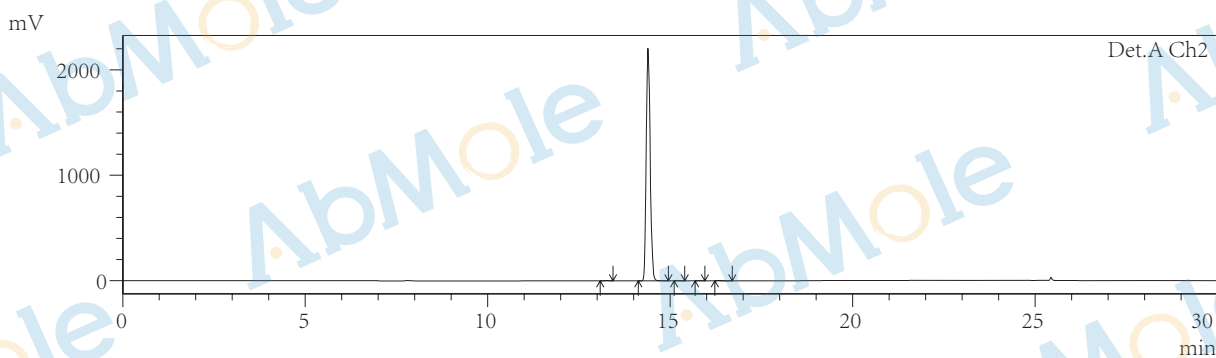


HPLC Report

Column : Inertil ODS-3 , 5um 4.6*150mm
 Mobile phase : Solvent A: H2O(0.05%H3PO4) Solvent B:ACN(0.05%H3PO4)
 Temperature : 40 °C
 Flow rate : 1mL/min
 Run time : 3min gradient(20%B), 12min gradient (20% -50%B), 5min gradient (50%-95%B),3 min(95%B),th
 Detector : UV
 Wavelength : 220/254 nm
 User name : AX-024 hydrochloride-01
 Notebook page :
 Sample description : AX-024 hydrochloride-01
 Injection Volume : AX-024 hydrochloride-01

Data File Name : AX-024 hydrochloride-01.lcd
 Method File Name : AX-024 hydrochloride-01.lcm
 Batch File Name : 20190627.lcb
 Data Acquired : 2019-6-27 9:44:44
 Data Processed : 2018-6-27 11:28:03

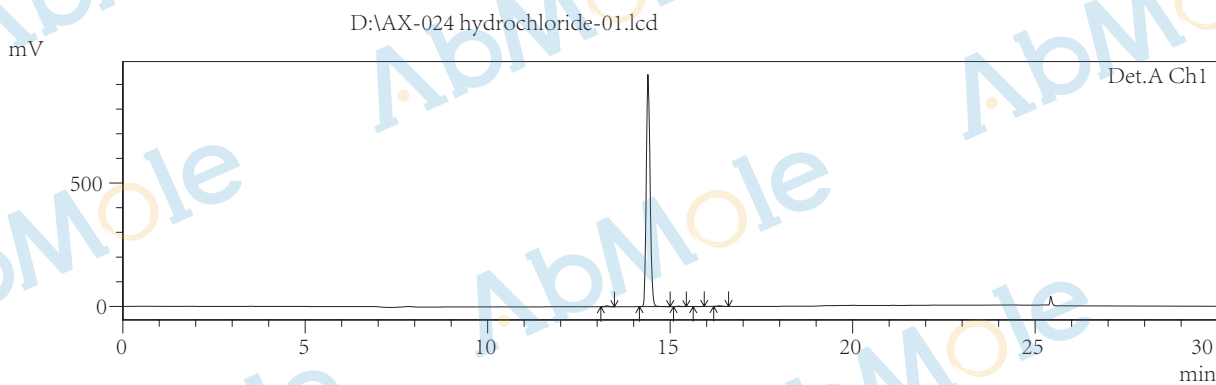

1 Det.A Ch1/220nm
2 Det.A Ch2/254nm

PeakTable

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Area %	Theoretical Plate
1	13.259	27090	0.391	59583.627
2	14.389	6865216	99.112	79848.581
3	15.232	11029	0.159	94645.781
4	15.784	3238	0.047	107196.759

Peak#	Ret. Time	Area	Area %	Theoretical Plate #
5	16.347	20143	0.291	90997.180
Total		6926716	100.000	

PeakTable

Detector A Ch2 254nm

Peak#	Ret. Time	Area	Area %	Theoretical Plate #
1	13.257	30422	0.181	62619.207
2	14.390	16704435	99.557	75485.136
3	15.233	13025	0.078	102321.170
4	15.780	10095	0.060	100055.206
5	16.348	20761	0.124	90918.285
Total		16778738	100.000	

*** End Of Report ***