
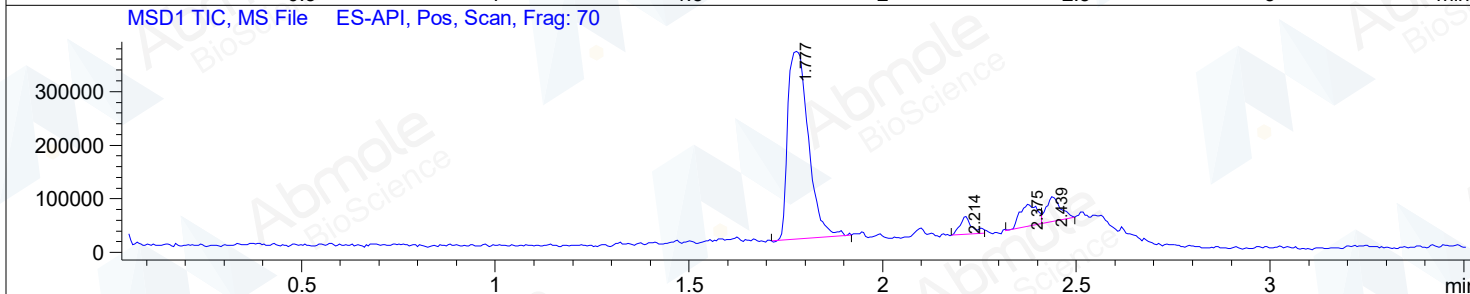
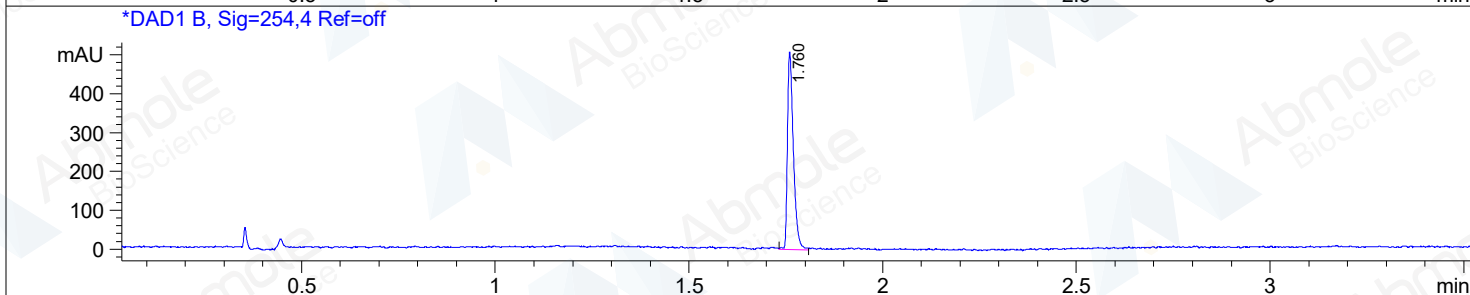


File D:\DATA
Injection Date : 28 Oct 18 5:38 pm +0800 **Tgt Mass (EZX)** :
Sample Name : FG-4592-02 **Location** : P1-F-02
Acq. Operator : LCMS **Inj** : 1
Spec. Reported : MS Integration **Inj Volume** : 4 ul
Acq. Method : D:\METHODS\1-POS-3MIN.M
Analysis Method : D:\METHODS\1-POS-3MIN.M
Sample Info : Easy-Access Method: '1-POS-3min'
Method Info : Mobile Phase: A: water(10mM Ammonium hydrogen carbonate) B: ACN
Gradient: 5%-95% B in 1.5min
Flow Rate: 2.0ml/min
Column: XBridge C18, 4.6*50mm, 3.5um
Oven Temperature: 40 C
MASS Range:110-800

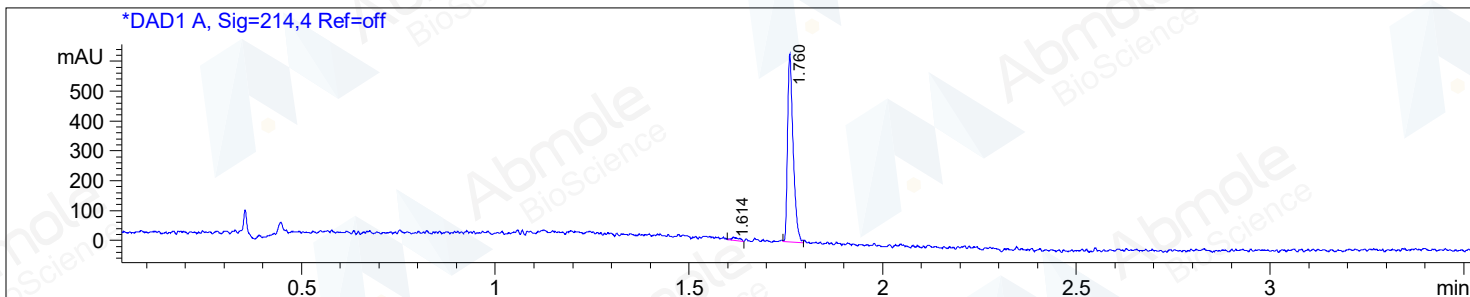

Integration Results for DAD1 A, Sig=214,4 Ref=off



RetTim	Width	Area	Height	Area%
1.61	0.02	7.97	7.67	0.31
1.76	0.02	633.74	628.84	99.69

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.76	0.02	547.71	509.01	100.00

Ret. Time: 1.78 <<<< POSITIVE SPECTRA >>>>

Ret. Time: 2.21

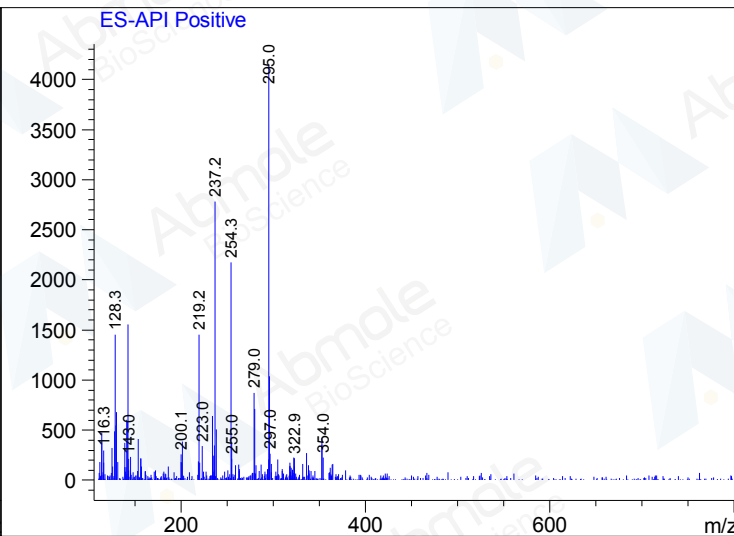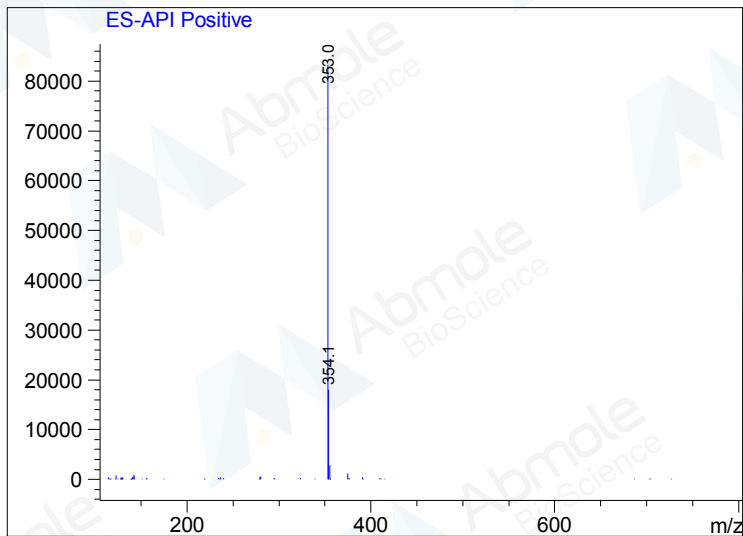

Ret. Time: 2.38

Ret. Time: 2.44

