




Current Data Parameters  
NAME Flumazenil-01  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190908  
Time\_ 13.26  
INSTRUM spect  
PROBHD 5 mm PADUL 13C  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 199.46  
DW 62.400 usec  
DE 6.50 usec  
TE 0 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 400.1324710 MHz  
NUC1 1H  
P1 10.00 usec  
PLW1 20.00000000 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

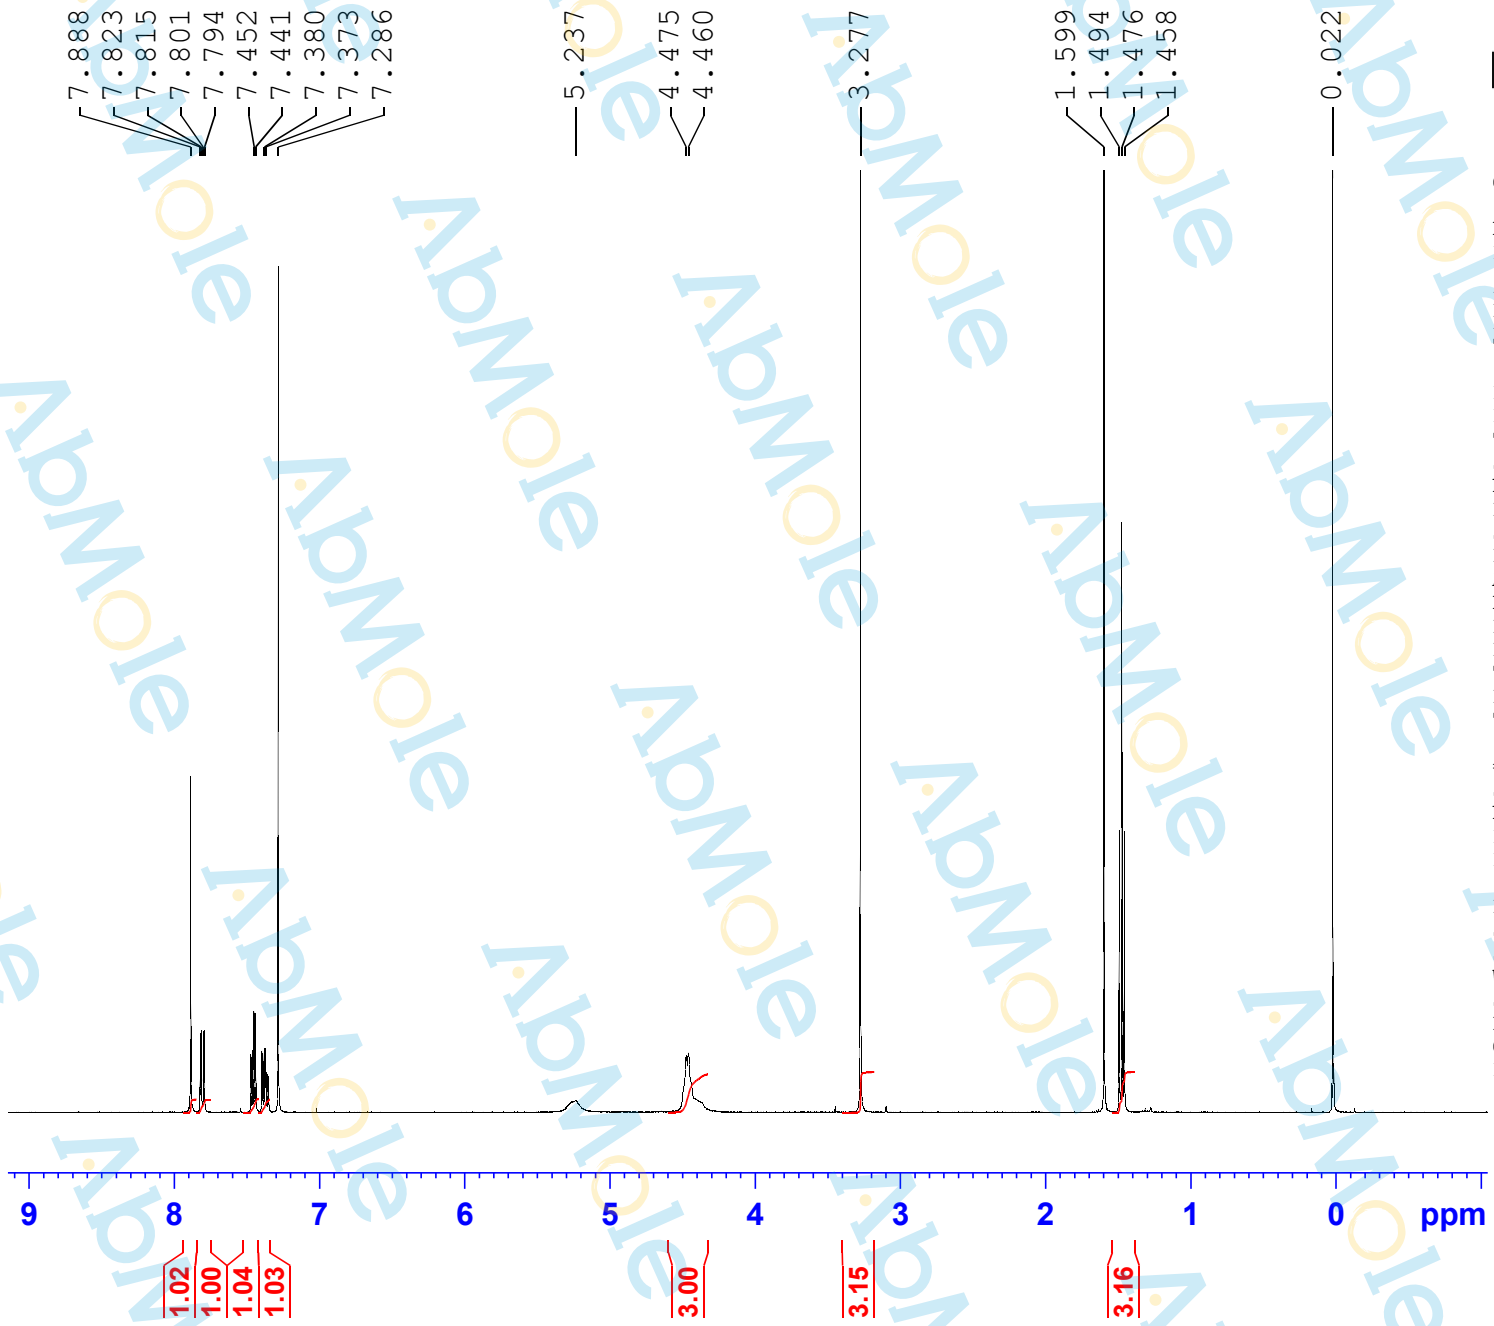

7.888  
7.823  
7.815  
7.801  
7.794  
7.452  
7.441  
7.380  
7.373  
7.286

5.237  
4.475  
4.460

3.277

1.599  
1.494  
1.476  
1.458

0.022

9 8 7 6 5 4 3 2 1 0 ppm

1.02  
1.00  
1.04  
1.03

3.00

3.15

3.16