

8.632
8.304
8.297
8.282
8.275
7.866
7.696
7.674
7.651
7.454
7.435
7.415
7.285
7.266
7.248
7.229

1.586
0.024




Current Data Parameters
NAME GW9662-03
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190325
Time_ 12.40
INSTRUM spect
PROBHD 5 mm PADUL 13C
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 8
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 199.46
DW 62.400 usec
DE 6.50 usec
TE 297.3 K
D1 1.00000000 sec
TD0 1

==== CHANNEL f1 =====
SFO1 400.1324710 MHz
NUC1 1H
P1 10.00 usec
PLW1 20.00000000 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

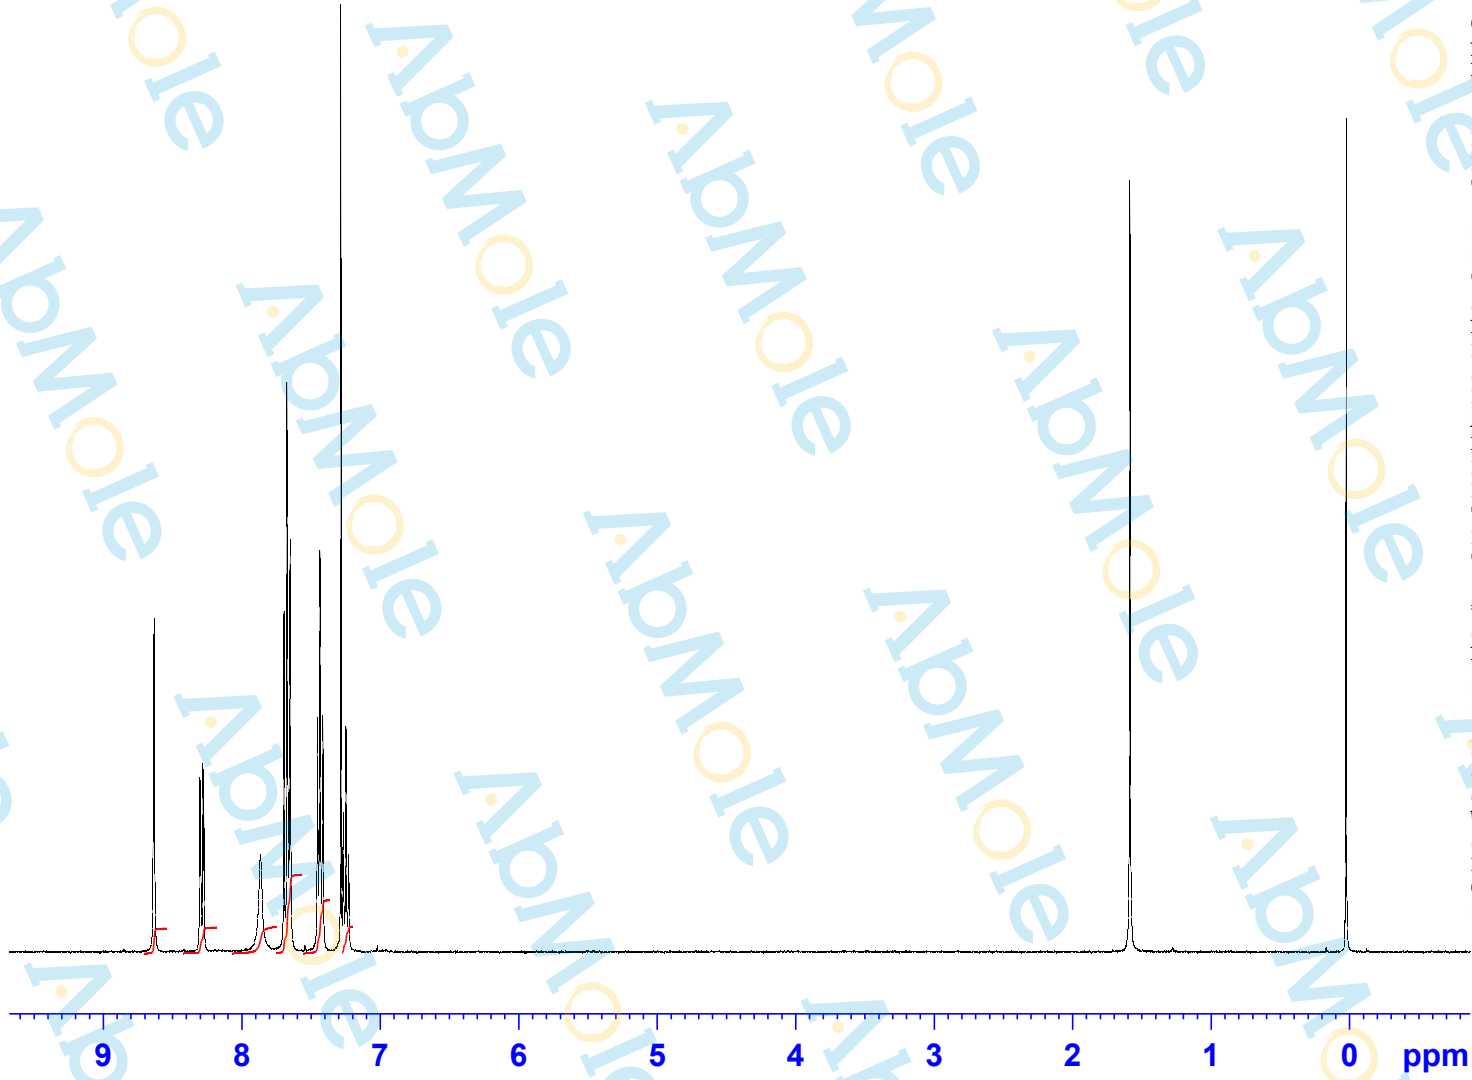

1.00
1.05
1.08
3.17
2.15
1.09

9 8 7 6 5 4 3 2 1 0 ppm