



7.308  
7.285  
7.276  
7.247  
7.227  
7.159  
7.140  
7.088  
7.068  
6.992  
6.990  
6.986  
6.971  
6.965


3.856  
2.447  
2.111  
1.575

0.033  
0.025  
0.017

Current Data Parameters  
NAME J 147-01  
EXPNO 1  
PROCNO 1  
  
F2 - Acquisition Parameters  
Date\_ 20181217  
Time\_ 14.17  
INSTRUM spect  
PROBHD 5 mm PADUL 13C  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 8  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 199.46  
DW 62.400 usec  
DE 6.50 usec  
TE 296.1 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 400.1324710 MHz  
NUC1 1H  
P1 10.00 usec  
PLW1 20.00000000 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

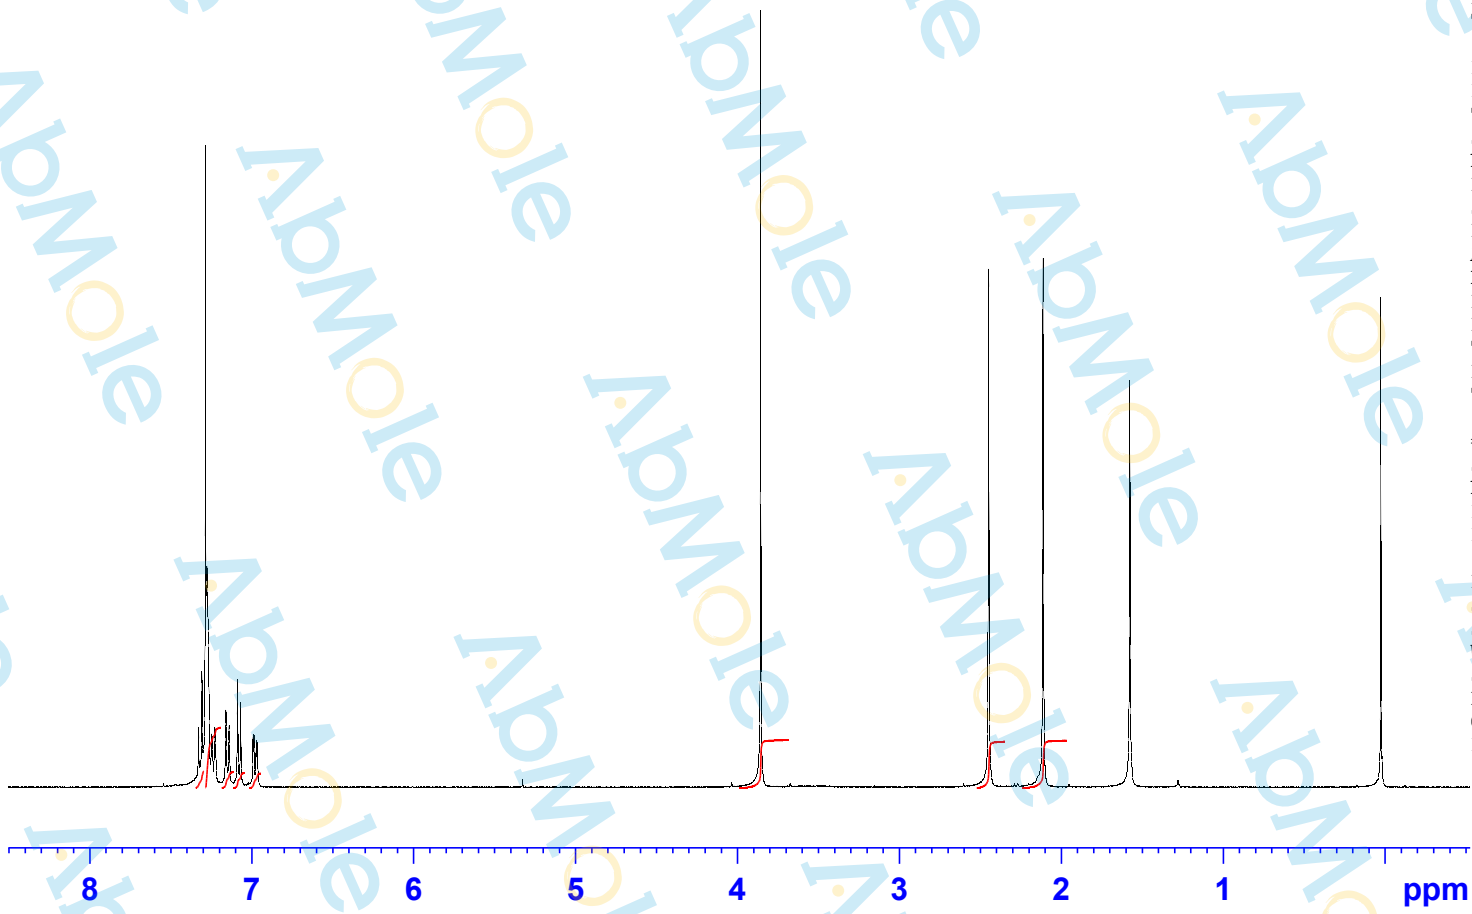

1.13  
4.02  
1.07  
1.00  
0.97

3.19

3.08  
3.14

8 7 6 5 4 3 2 1 ppm