
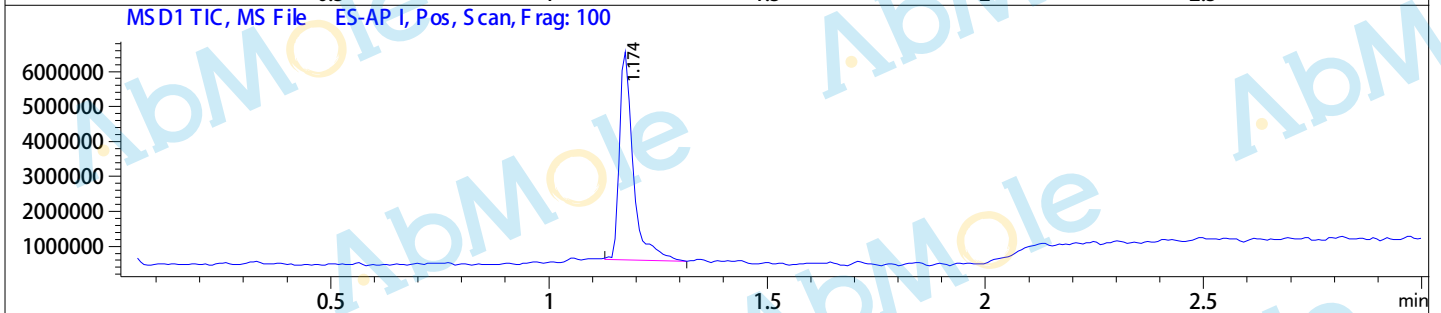



LC/MS Report

Injection Date : 30 Mar 21
 Sample Name : Ki20227-01

Method Info : Mobile Phase : A:water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient:5%B increase to 95%B within 1.5min,95%B for 1.5min
 Flow Rate :2.0ml/min
 Column :SunFire C18 3.5um, 4.6mm*50mm
 Column Temperature:50C
 Detection:UV(214nm,4nm) and MS(ESI,POS Mode,110-1300amu)



Integration Results for DAD1 A, Sig=2144 Ref=off

RetTim	Width	Area	Height	Area%
1.11	0.01	26.97	28.09	1.60
1.17	0.01	1658.25	1932.88	98.40

Integration Results for DAD1 B, Sig=2544 Ref=off

RetTim	Width	Area	Height	Area%
1.17	0.01	1794.40	2062.78	100.00

Ret. Time: 1.17 <<<< POSITIVE SPECTRA >>>>

