


```
=====
Acq. Operator   : System                               Seq. Line :    2
Acq. Instrument : LC1260                               Location  : Vial 11
Injection Date  : 5/13/2016 3:09:51 PM                Inj       :    1
                                                    Inj Volume:    0 µl
Different Inj Volume from Sequence !   Actual Inj Volume :    2 µl
Acq. Method    : E:\DATA\Data\20160511\20130913-01 2016-05-13 14-43-25\10-90 AC
               15MIN.M
Last changed   : 5/13/2016 2:43:26 PM by System
Analysis Method: D:\PUBLIC\20160512\20160127 2016-05-13 15-34-12\LLH-4.D\DA.M (5-95 6MIN.M)
Last changed   : 4/28/2016 10:48:55 AM
=====
```

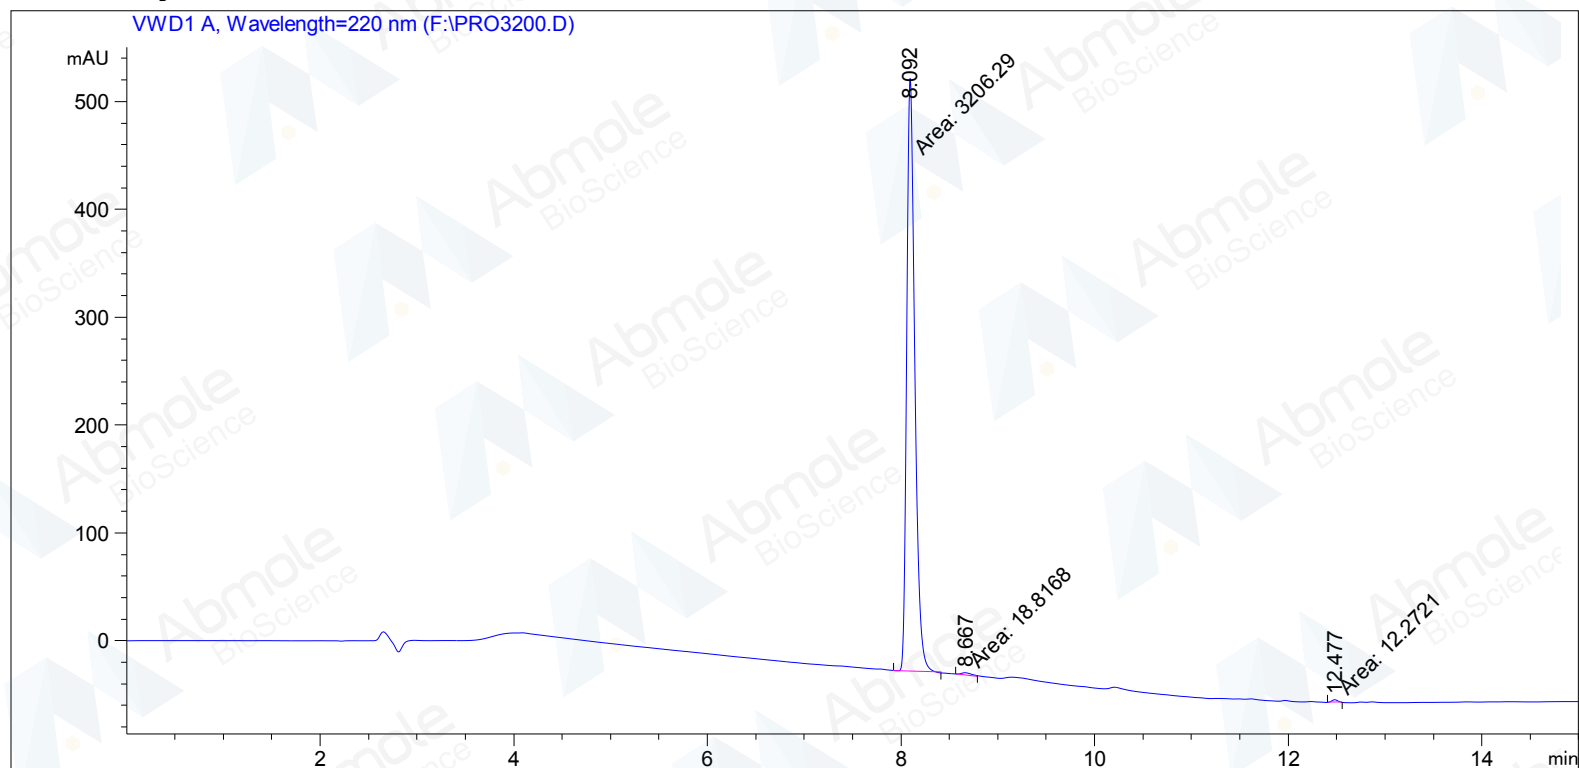

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=220 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.092	MM	0.0971	3206.29468	550.55023	99.0397
2	8.667	MM	0.1343	18.81678	2.33511	0.5812
3	12.477	MM	0.0771	12.27214	2.65312	0.3791

Totals : 3237.38360 555.53846

=====
*** End of Report ***