

Data file:

C:\CHEM32\1\DATA\M10035-Semagluti de-01Final.D
M10035-Semagluti de-01

Sample name:

Mobile phase: Buffer A: 0.1%TFA in H2O

Description:

Buffer B: 0.1%TFA in ACN
Gradient: 42-52% B in 20min , Flow rate: 1.0ml/min
Column: phenomenex C18, 4.6*150mm, 5um 100A (A-007)
Instrument: Agilent HPLC 1100

Instrument:

1100

Location:

24

Injection:


1 of 1

Injection volume:

10.000

Acq. operator:

QC

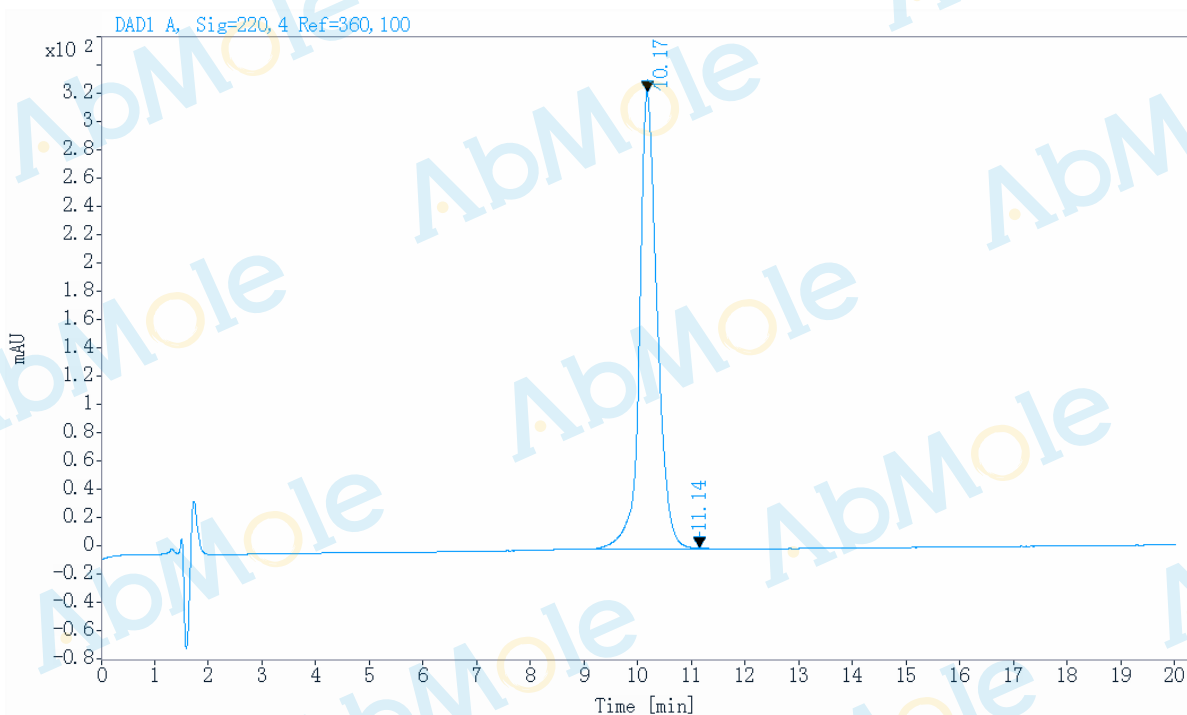

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
10.170	MF	0.3837	7458.8530	323.9824	99.8850	
11.140	FM	0.1949	8.5884	0.7344	0.1150	
Sum			7467.4414			