

M10287-GSK547-01-LCMS

Sample Information

LCMS


Acquired by : System Administrator
Sample Name : M10287-GSK547-01
Method File : B 5%-95%-P-new - 2.6min.lcm

Date Acquired : 2021/7/17 10:19:12
Injection Volume : 3
Vial : 27


Column : Waters SunFire C18 50*4.6mm 5um 2.000ml/min 2.6min
Pump A : 0.1% FA and 10% ACN in H2O
Pump B : 0.1% FA and 10% H2O in ACN

Chromatogram


mAU

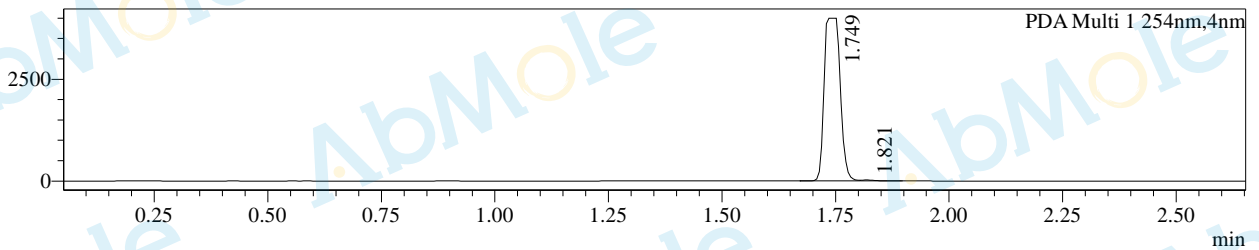

mAU

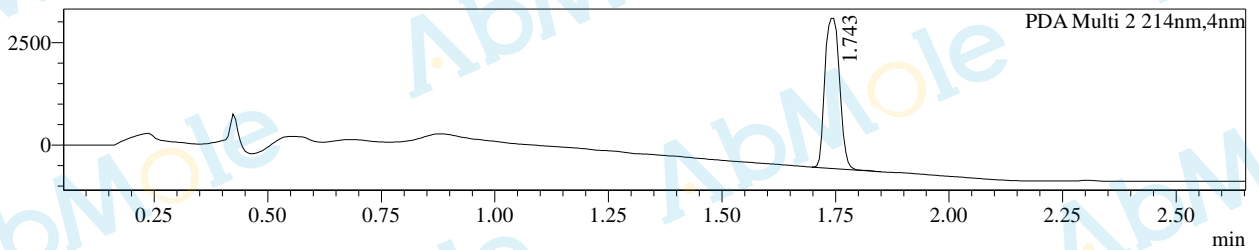

段号1

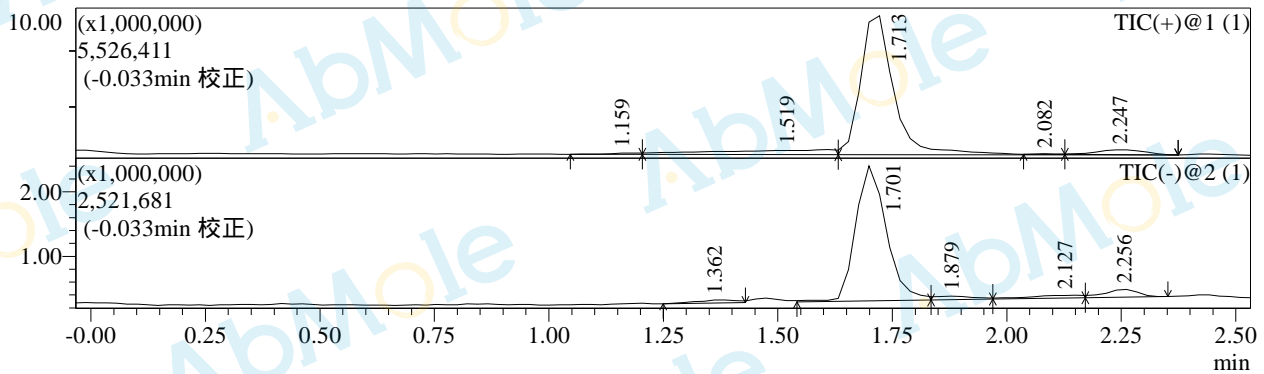

Integration Results for DAD

PDA Ch1 254nm


Peak#	Ret. Time	Height	Area	Area%
1	1.749	3996479	9750805	99.604
2	1.821	21526	38809	0.396
总计		4018005	9789614	100.000

PDA Ch2 214nm


Peak#	Ret. Time	Height	Area	Area%
1	1.743	3659791	8275996	100.000
总计		3659791	8275996	100.000

Mass Spectrum


Rt=1.159min 正

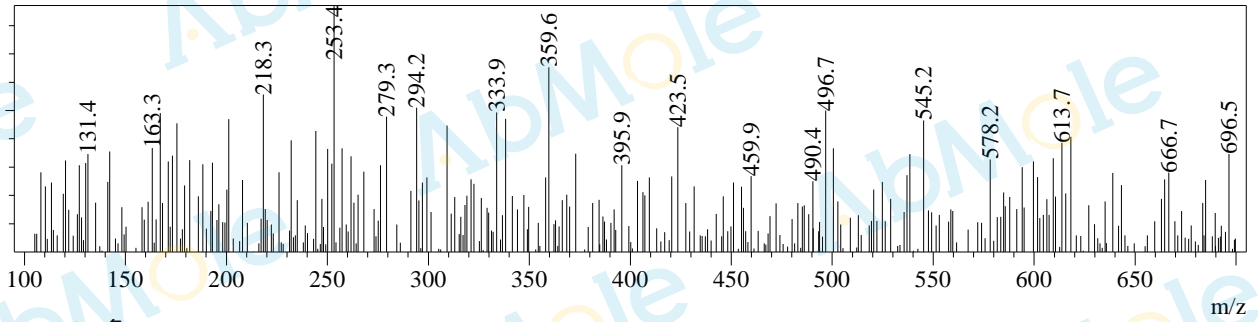


Rt=1.367min 负

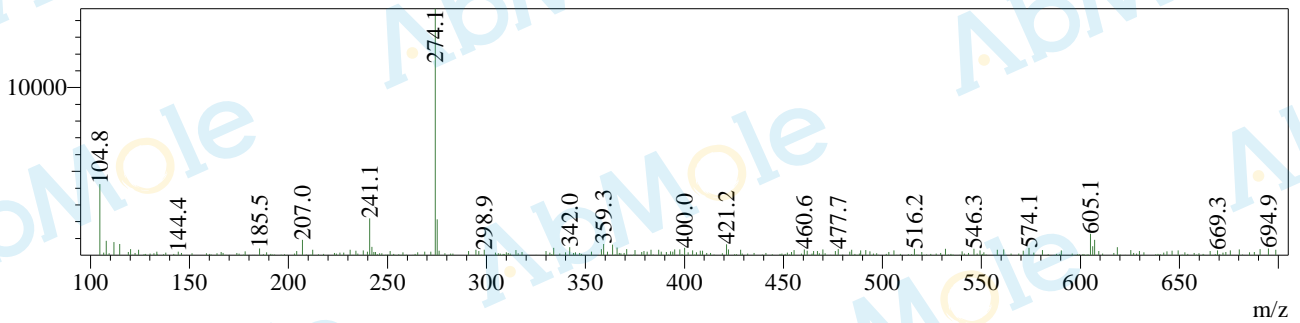


Rt=1.519min 正

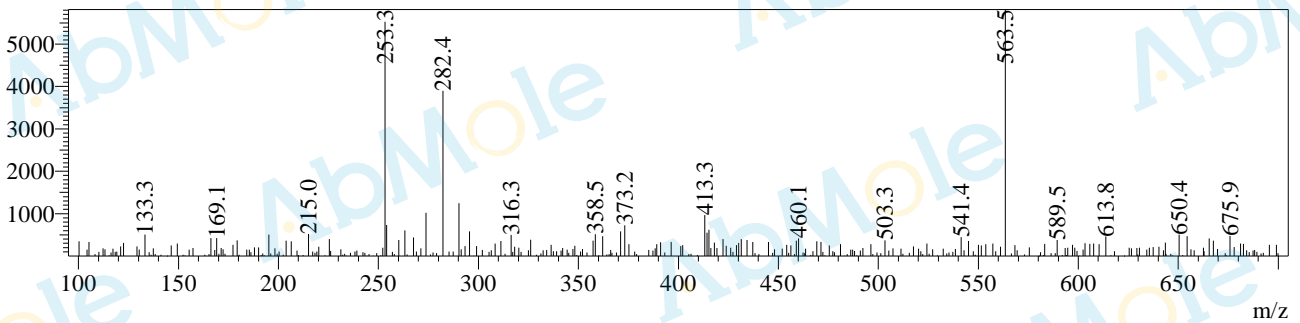


Rt=1.705min 负

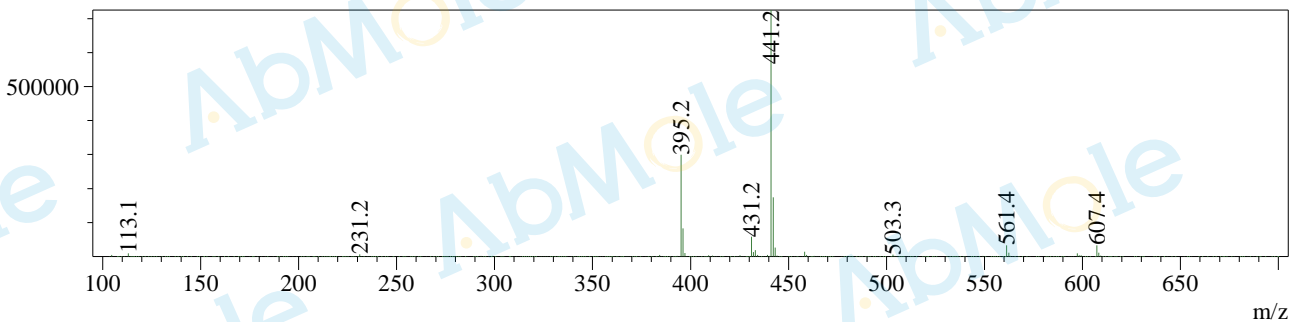


Rt=1.699min 正

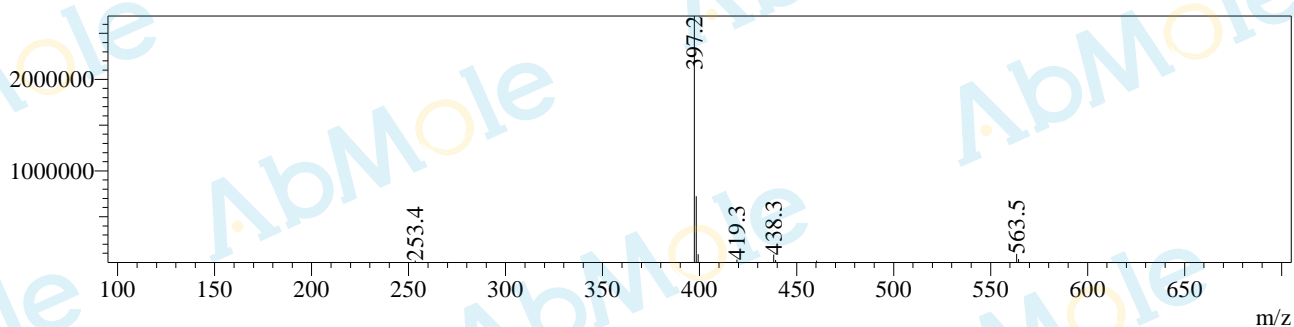


Rt=1.885min 负

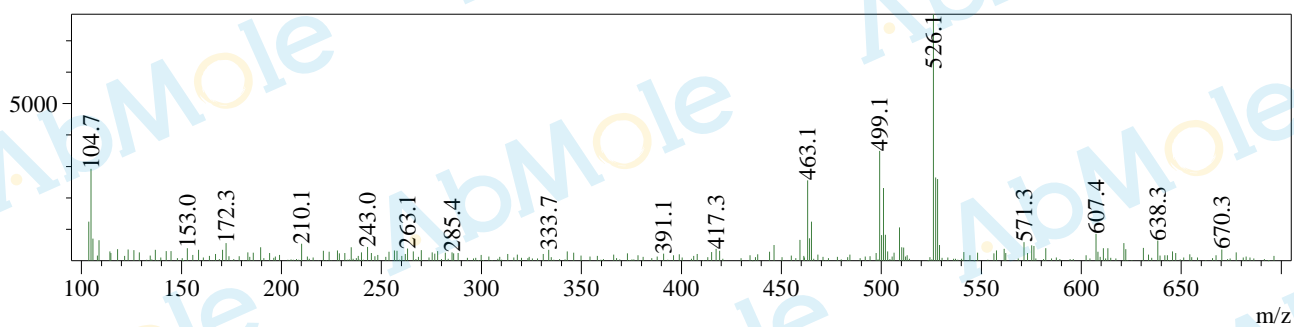


Rt=2.082min 正

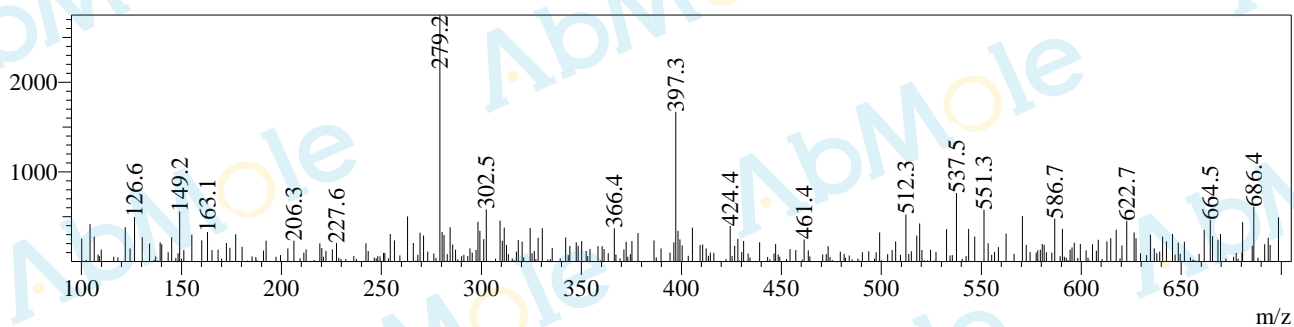

Rt=2.132min 负

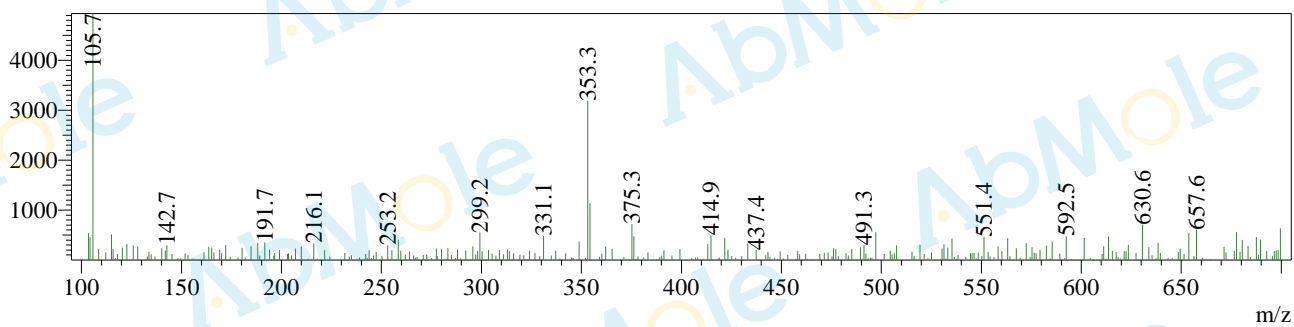

Rt=2.239min 正

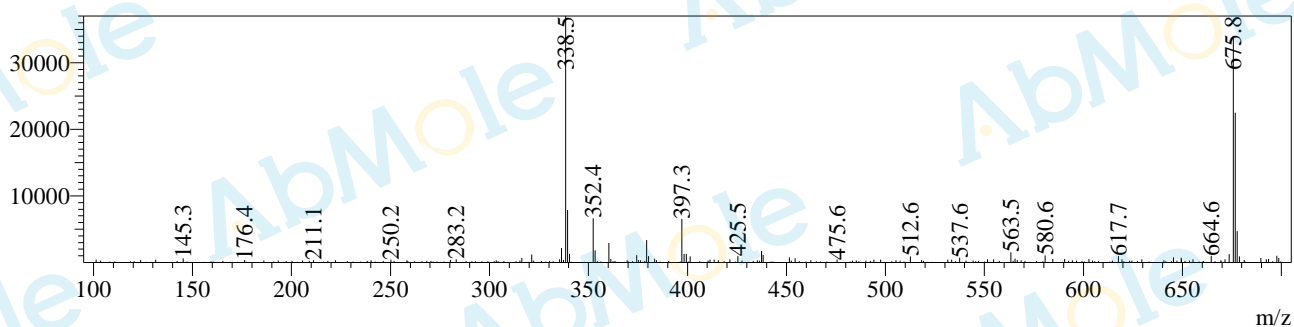

Rt=2.245min 负

