


```

=====
Acq. Operator   : admin
Sample Operator : 1
Acq. Instrument : 3
Sample Name    : M10423-DT2216-03
Location       : P1-B-08
Inj            : 1
Inj Volume     : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 5.000 µl
=====

```

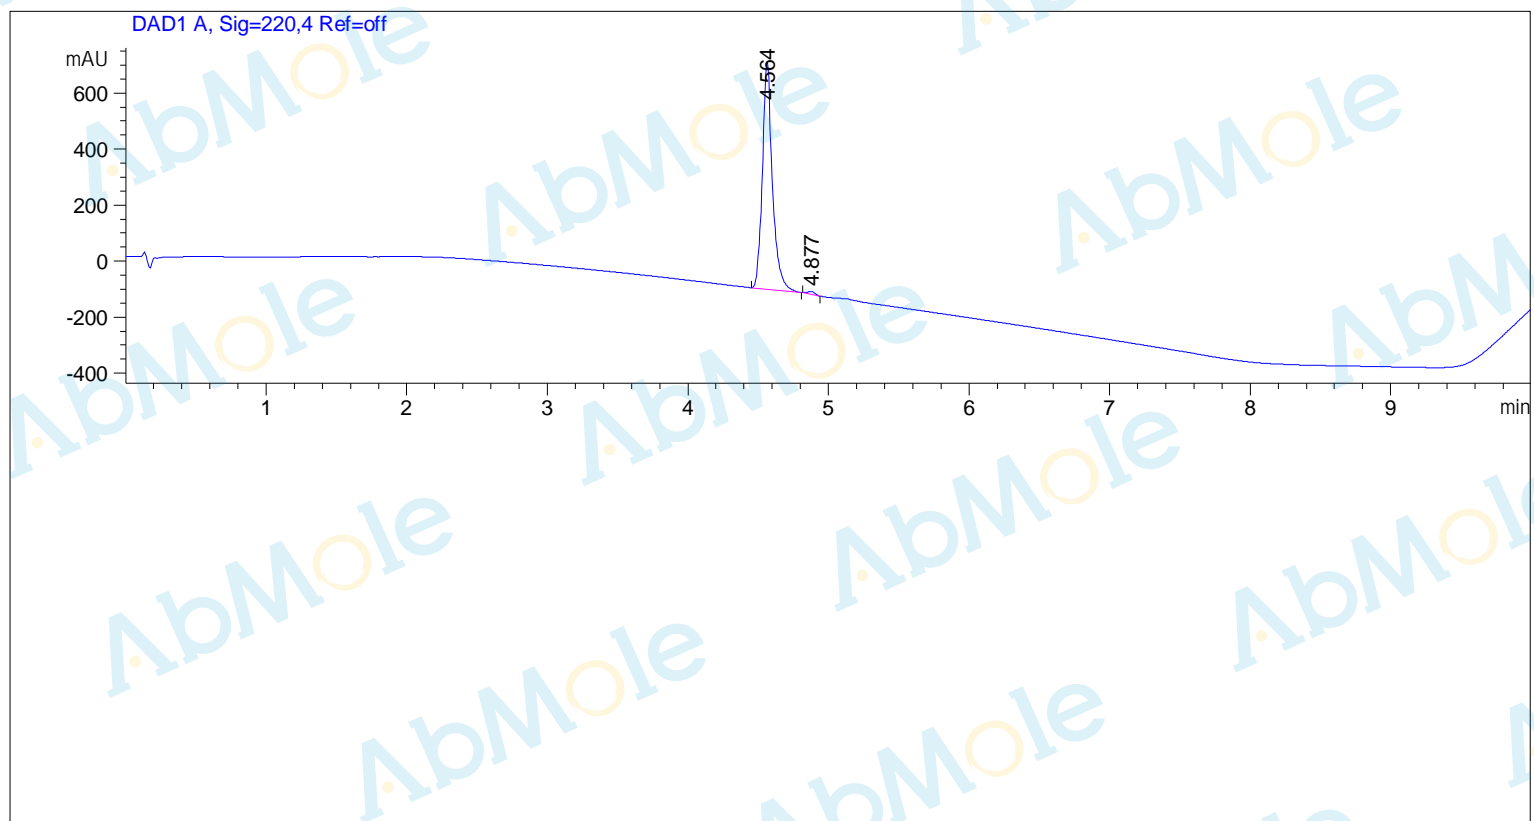

=====
Area Percent Report
=====

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.564	BB	0.0717	4020.19775	813.44110	99.1133
2	4.877	BB	0.0530	35.96577	10.23019	0.8867

Totals :

4056.16353 823.67129