


# MASS SPECTROMETRY REPORT

A: 4103.28±1.21

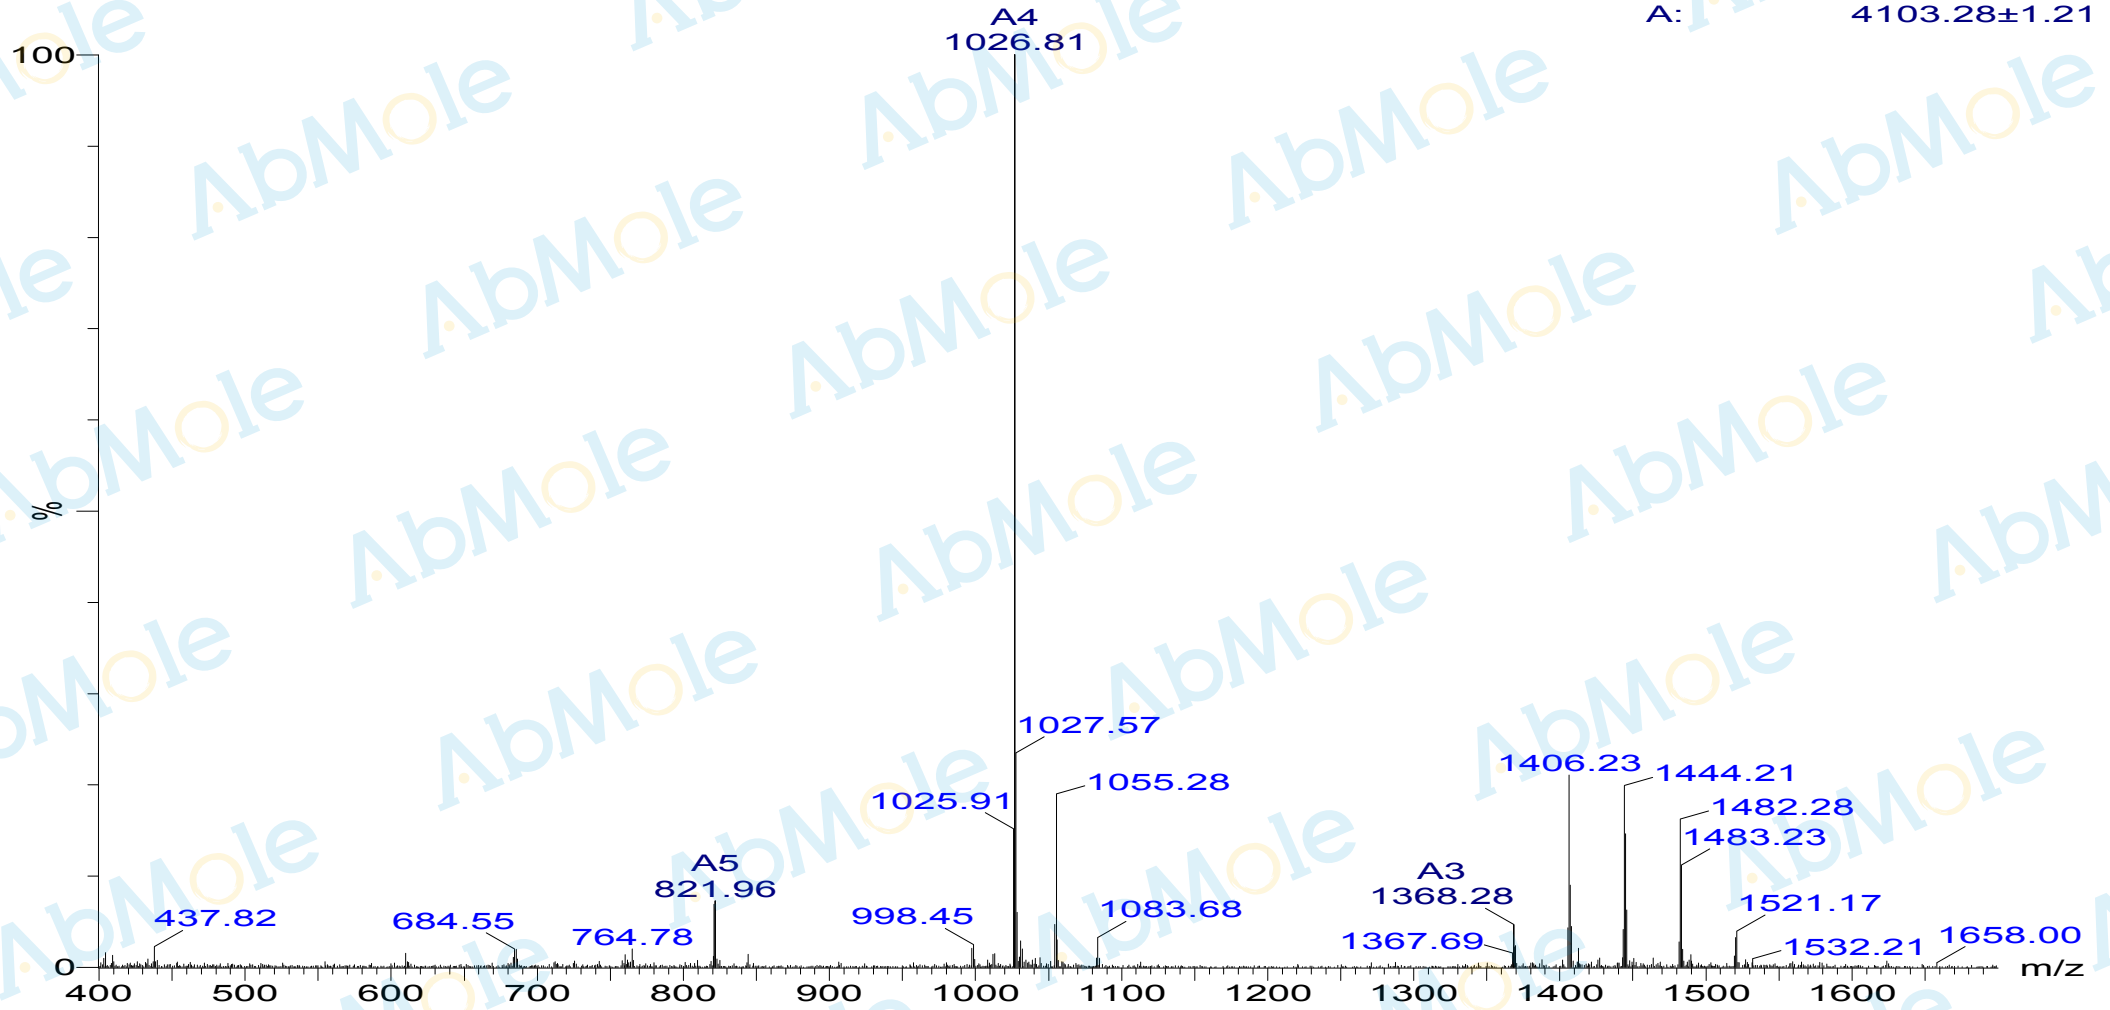

## Sample Description

Analyst: SHAO  
Sample: M10742-Vosoritide acetate-01  
M.W.: 4102.8  
Lot. No.:

## Instrument

Probe: Waters 2695  
Nebulizer Gas Flow: ESI  
CDL: 1.5L/min  
CDL Temp.: -20.0v  
Block Temp.: 250 °C  
200 °C

## Waters 2695

Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.5ml/min  
B. Conc.: 50%H2O/50%ACN