


=====
 Acq. Operator : SYSTEM
 Acq. Instrument : 0
 Sample Name : M10953-MRTX-1719-02

Seq. Line : 1
 Location : P2-B-01
 Inj : 1
 Inj Volume : 1.000 µl

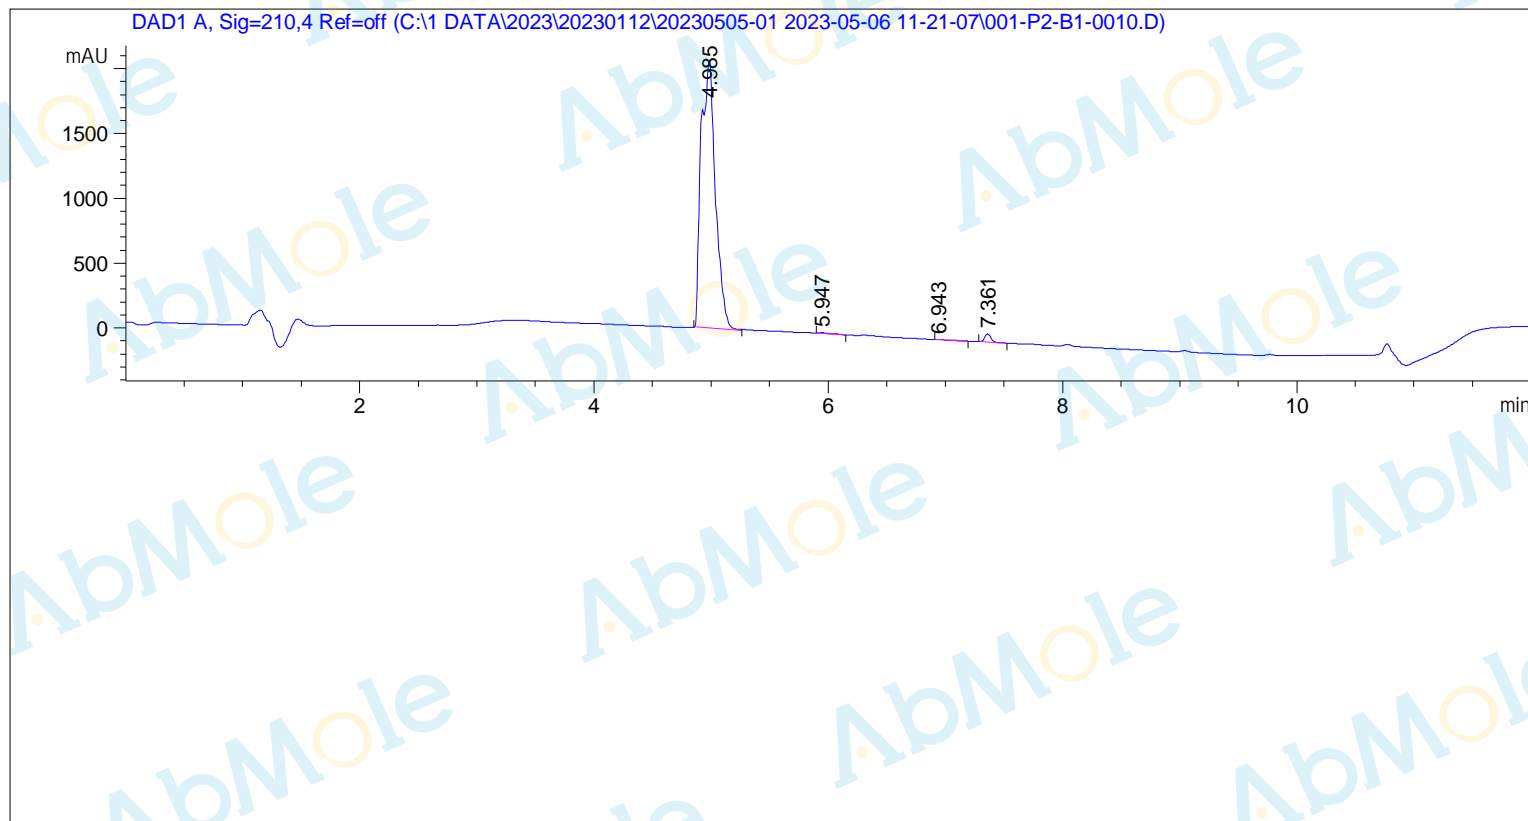

=====
 Area Percent Report
 =====

Sorted By : Signal
 Multiplier : 1.0000
 Dilution : 1.0000
 Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.985	MM	0.1405	1.74704e4	2071.79028	98.3834
2	5.947	BB	0.0903	45.00044	6.88527	0.2534
3	6.943	BB	0.0882	15.34546	2.41299	0.0864
4	7.361	BB	0.0568	226.71735	61.86798	1.2767

Totals : 1.77575e4 2142.95652