


```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    4
Acq. Instrument : 0                          Location  : P2-E-06
Sample Name     : M11555-Relacorilant-01     Inj       :    1
                                           Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl
=====

```

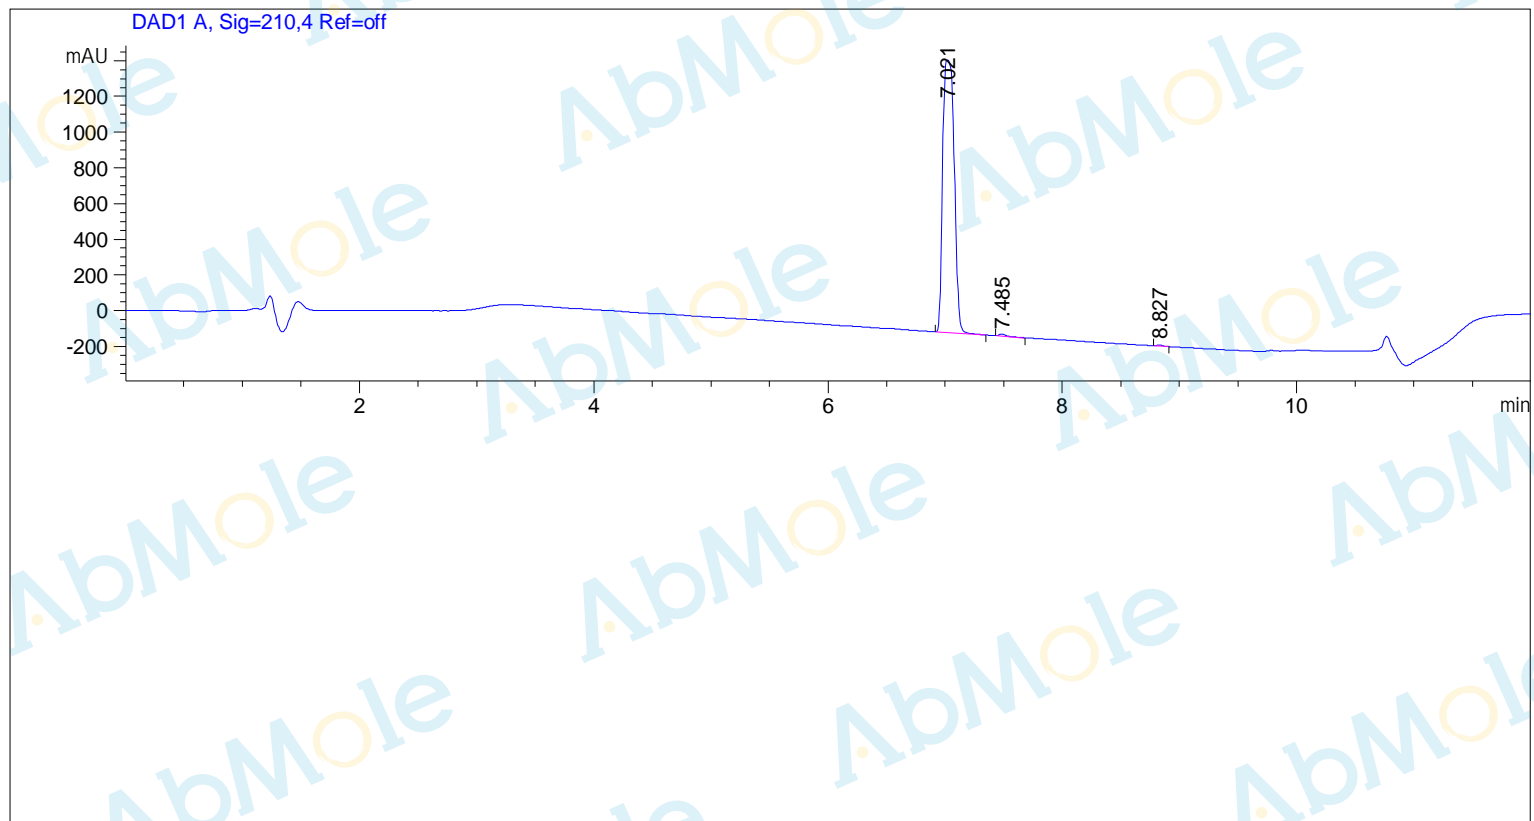

```

=====
                          Area Percent Report
=====

```

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution      :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	7.021	BB	0.1138	1.04383e4	1525.32666	99.5061
2	7.485	BB	0.0573	36.08270	10.19442	0.3440
3	8.827	BB	0.0585	15.72384	4.31898	0.1499

```
Totals :                1.04902e4  1539.84006
```