


=====
Acq. Operator : admin
Sample Operator : M14279-GSK205-01
Acq. Instrument : 3

Location : P1-B-06

Inj : 1

Inj Volume : 0.100 µl

Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

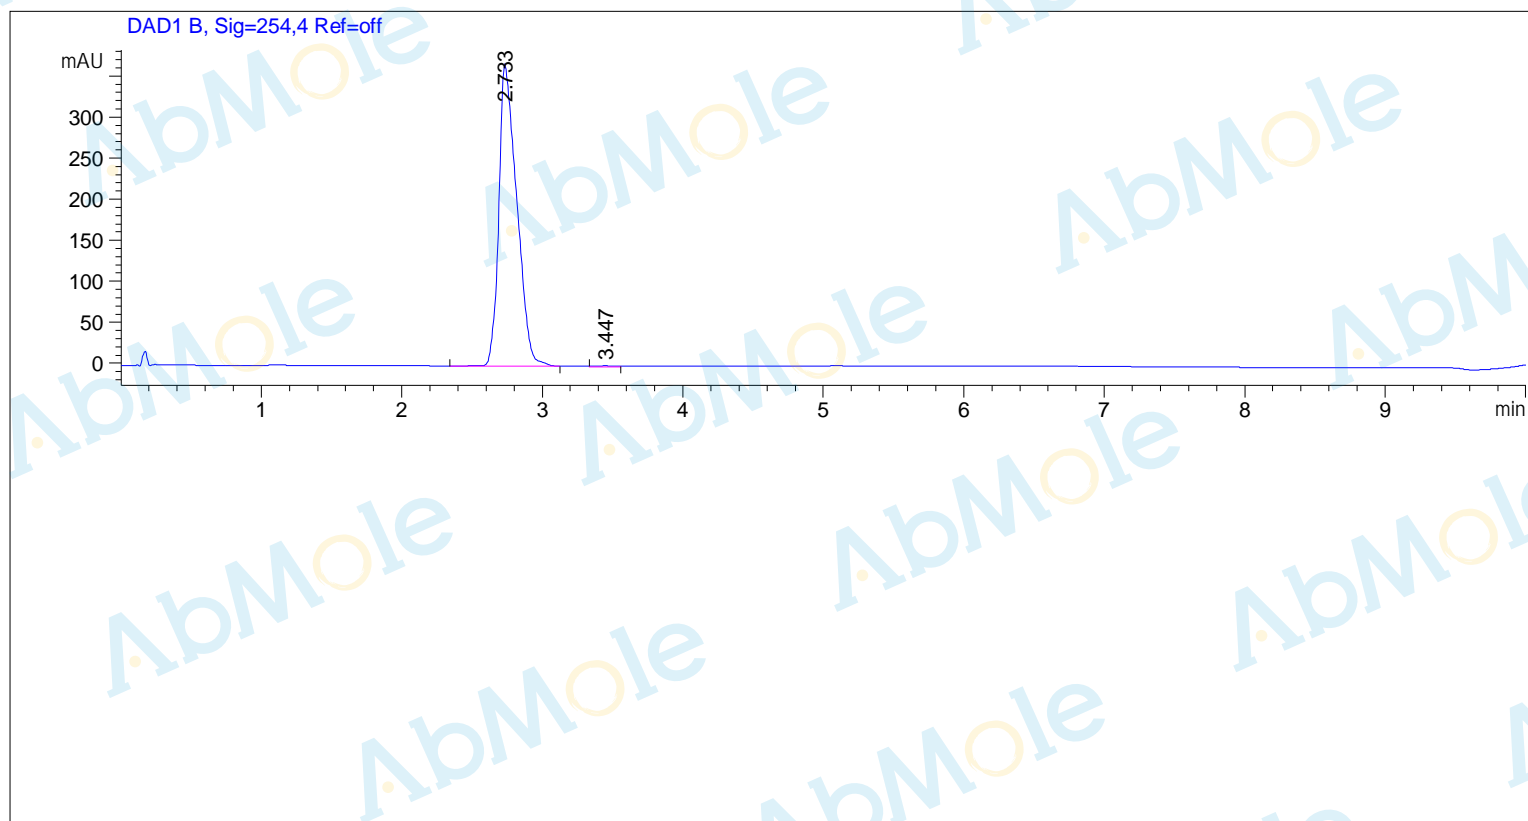

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.733	BB	0.1389	3238.66016	367.13400	99.7532
2	3.447	MM	0.1320	8.01362	1.01177	0.2468

Totals : 3246.67378 368.14578