




Sample name: M1894-Rosiglitazone-07  
Instrument: A011  
Inj. volume: 2  
Acq. method: HPLC  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

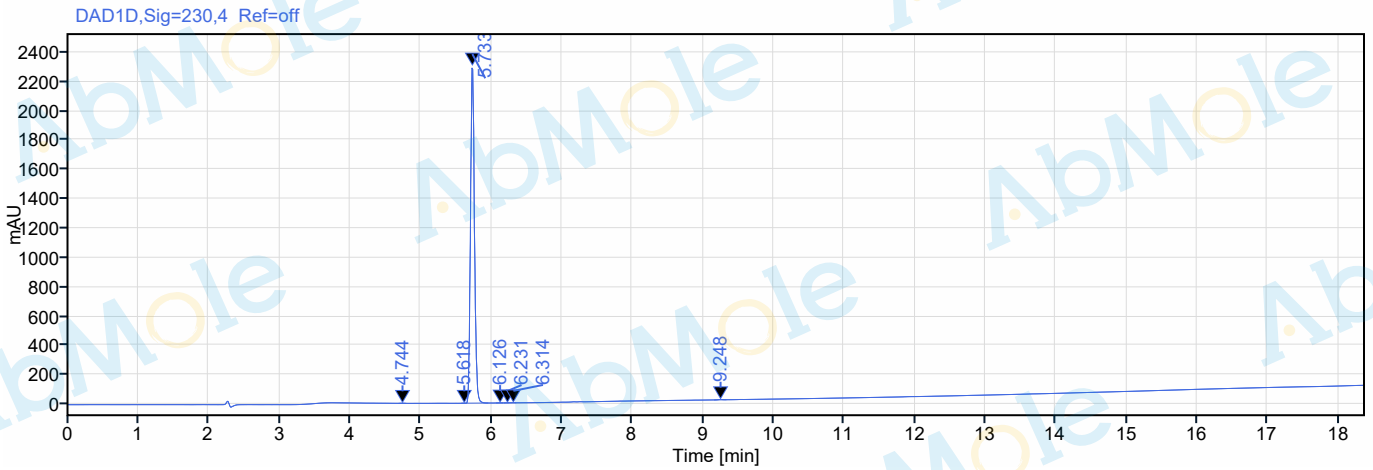

Signal: DAD1D,Sig=230,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%
4.744	BM m	0.11	3.25	1.10	0.04
5.618	MM m	0.07	1.03	0.43	0.01
5.733	BM m	0.31	8969.75	2299.26	99.82
6.126	MM m	0.10	1.57	0.50	0.02
6.231	MM m	0.08	0.58	0.20	0.01
6.314	MM m	0.09	1.67	0.57	0.02
9.248	BB	0.17	8.21	1.85	0.09