


=====
Acq. Operator : admin
Sample Operator : M1948-BI-D1870-04
Acq. Instrument : 3
Location : P2-D-09
Inj : 1
Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl

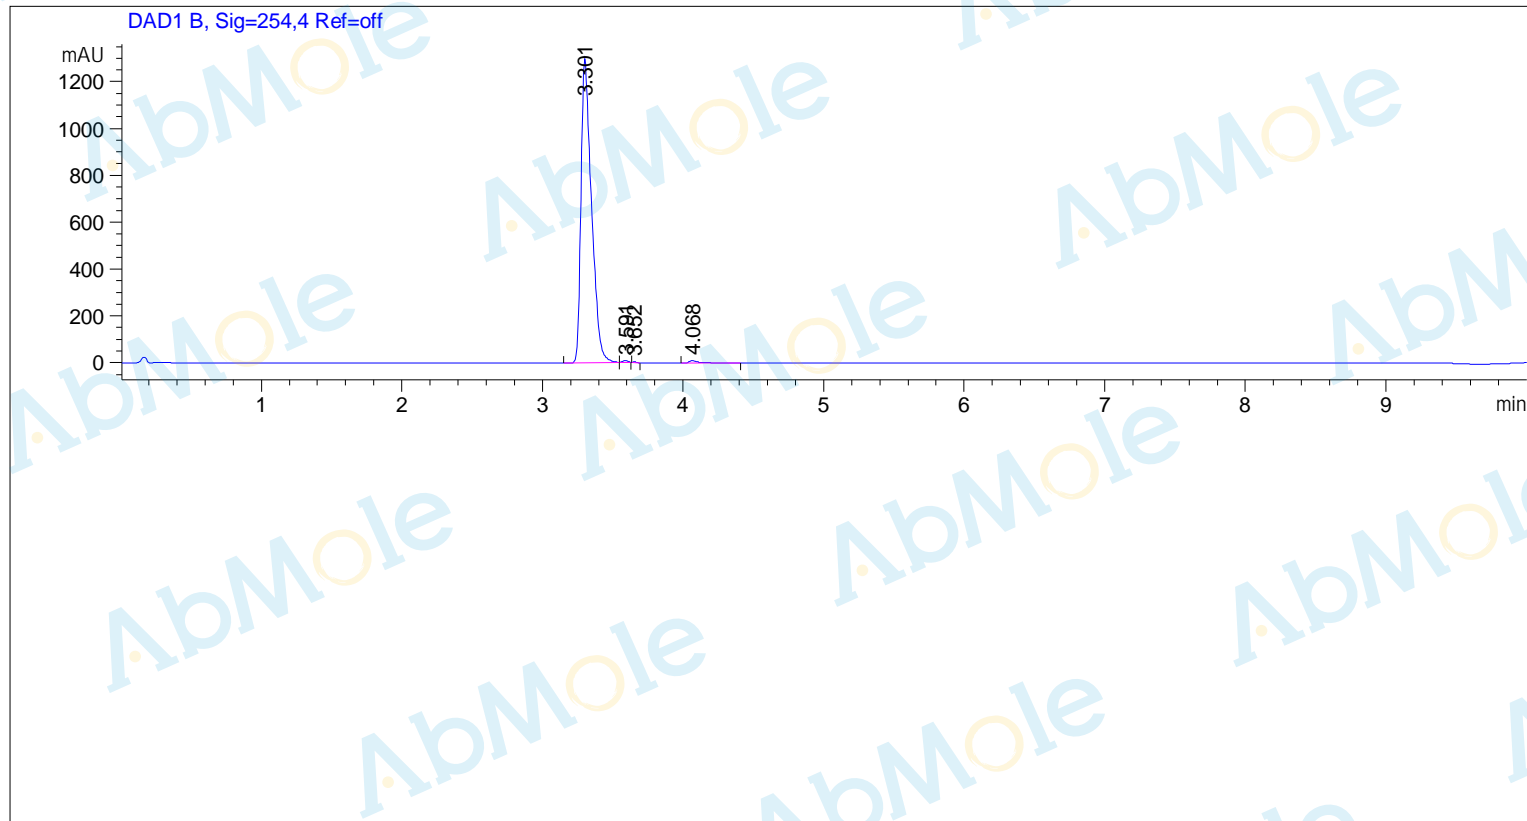

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.301	BB	0.0785	6744.36328	1299.77856	98.8310
2	3.591	BB	0.0399	18.77381	7.85718	0.2751
3	3.652	BB	0.0354	3.80821	1.75140	0.0558
4	4.068	BB	0.0772	57.18896	10.55069	0.8380

Totals : 6824.13427 1319.93784