




Sample name: M2026-AT-406-01
Instrument: A010
Inj. volume: 2
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

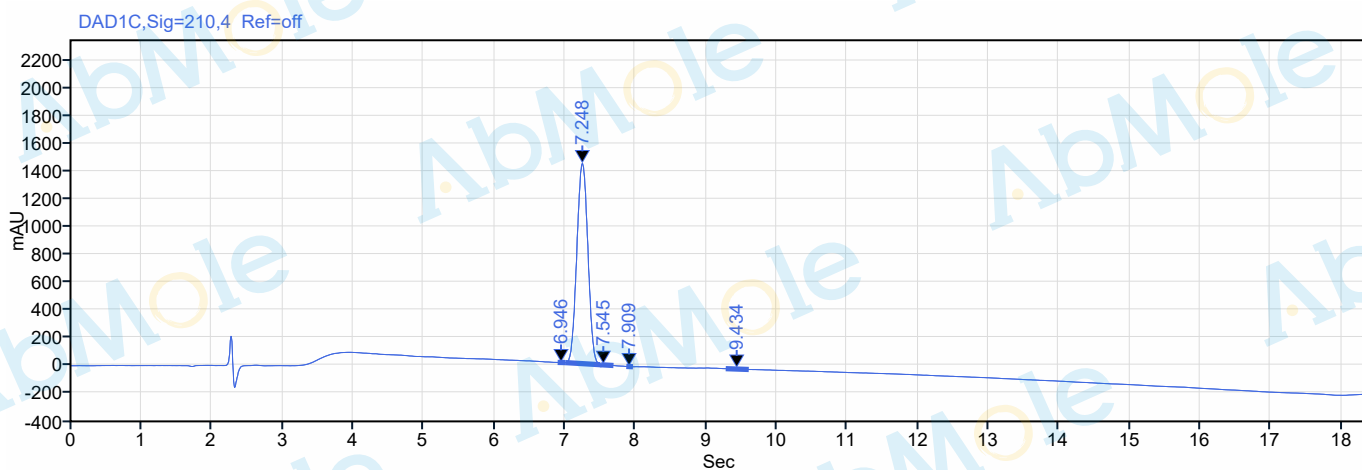

Signal: DAD1C,Sig=210,4 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
6.946		0.11	6.3	1.9	0.04
7.248		0.50	15700.3	1446.0	99.06
7.545		0.18	42.7	7.1	0.27
7.909		0.09	5.9	2.1	0.04
9.434		0.33	93.8	9.3	0.59