




Sample name: M2040-Bay 11-7082-02  
Instrument: A012  
Inj. volume: 5  
Acq. method: HPLC  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

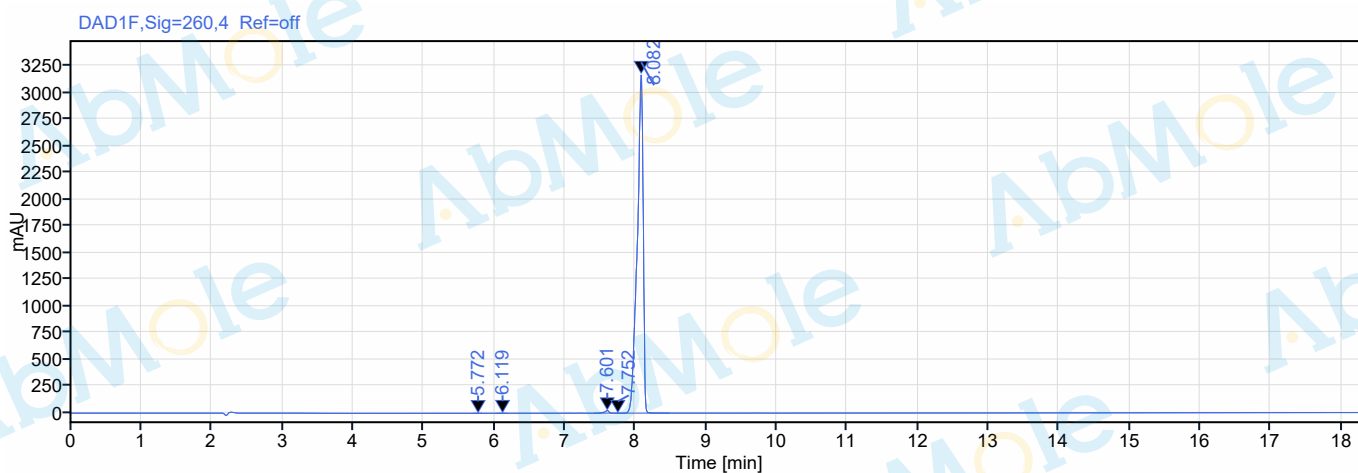

Signal: DAD1F,Sig=260,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%
5.772	MM m	0.13	0.81	0.23	0.00
6.119	BB	0.17	4.50	1.33	0.02
7.601	MB m	0.29	108.90	24.52	0.58
7.752	MM m	0.11	0.64	0.23	0.00
8.082	BM m	0.68	18741.50	3180.30	99.39