




Sample name: M2066-Staurosporine-07
Instrument: A010
Inj. volume: 4
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

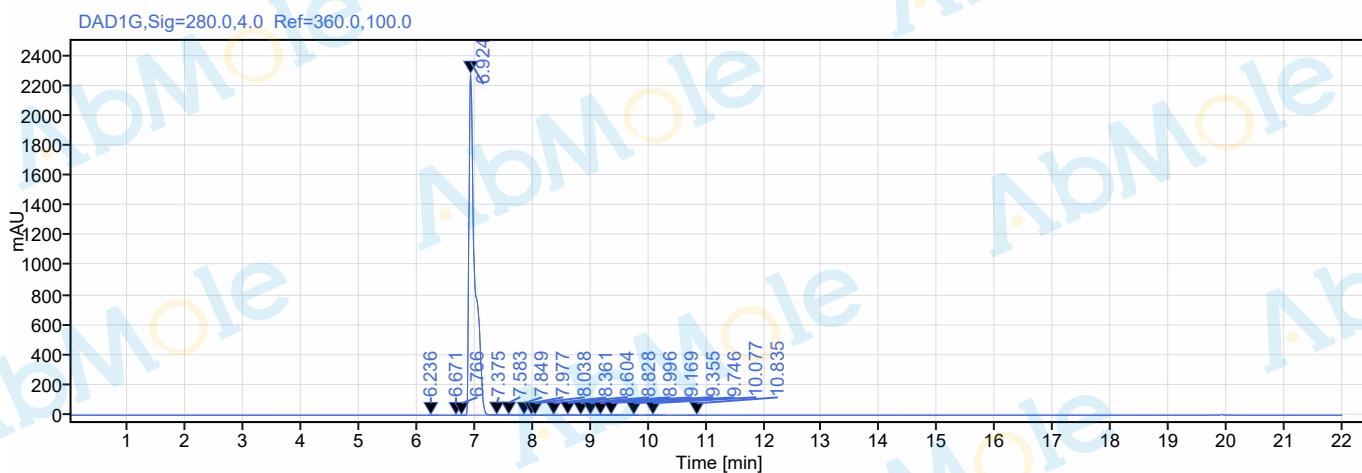

Signal: DAD1G,Sig=280.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
6.236	MM m	0.19	0.51	0.10	0.00
6.671	MM m	0.13	0.96	0.23	0.01
6.766	MM m	0.08	0.58	0.14	0.00
6.924	MM m	0.53	16224.47	2280.54	99.24
7.375	MM m	0.19	17.77	2.04	0.11
7.583	MM m	0.27	17.25	2.53	0.11
7.849	MM m	0.10	2.94	0.62	0.02
7.977	MM m	0.15	5.74	0.90	0.04
8.038	MM m	0.23	3.26	0.37	0.02
8.361	MM m	0.19	0.84	0.11	0.01
8.604	BM m	0.30	21.70	2.49	0.13
8.828	MM m	0.12	4.58	0.71	0.03
8.996	MM m	0.20	9.93	1.11	0.06
9.169	MM m	0.13	6.08	0.97	0.04
9.355	MM m	0.37	21.20	1.97	0.13
9.746	MM m	0.24	2.04	0.23	0.01
10.077	MM m	0.38	7.60	0.89	0.05
10.835	MM m	0.25	0.88	0.11	0.01