




Agilent Technologies

Sample name: M21004-Danicamtiv (MYK-491)-01
Instrument: 2
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

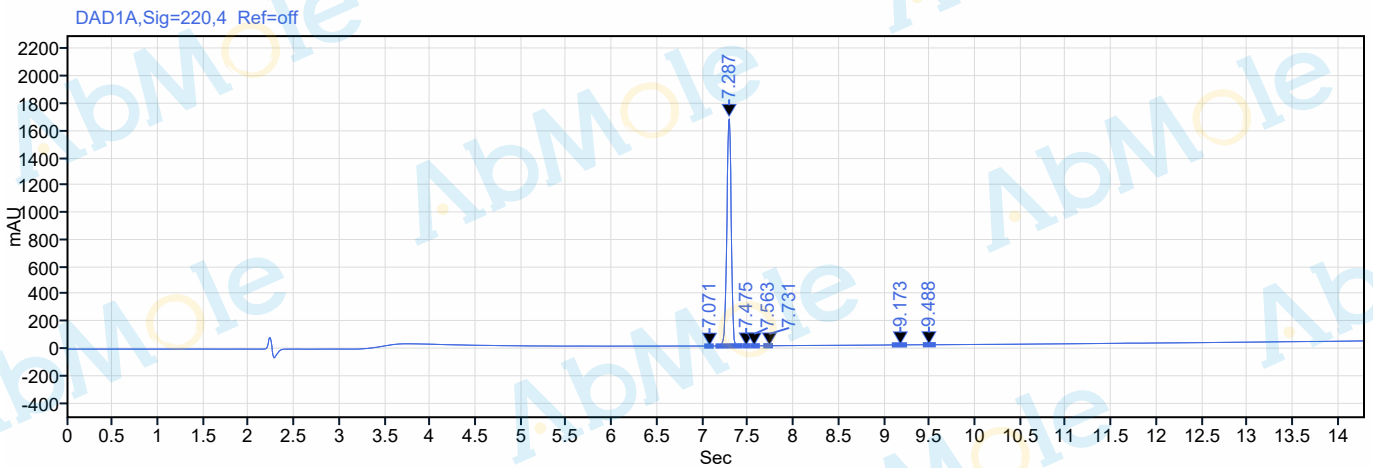

Signal: DAD1A,Sig=220,4 Ref=off

RT [min]	Area	Height	Area%
7.071	1.4	0.5	0.024
7.287		1680.3	99.684
7.475	1.0	0.4	0.018
7.563	0.6	0.2	0.010
7.731	0.7	0.2	0.012
9.173	7.8	1.9	0.139
9.488	6.3	1.7	0.112