


```

=====
Acq. Operator   : admin
Sample Operator : M2542-CTEP-01
Acq. Instrument : 3
Location       : P1-F-05
Inj            : 1
Inj Volume    : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl
=====

```

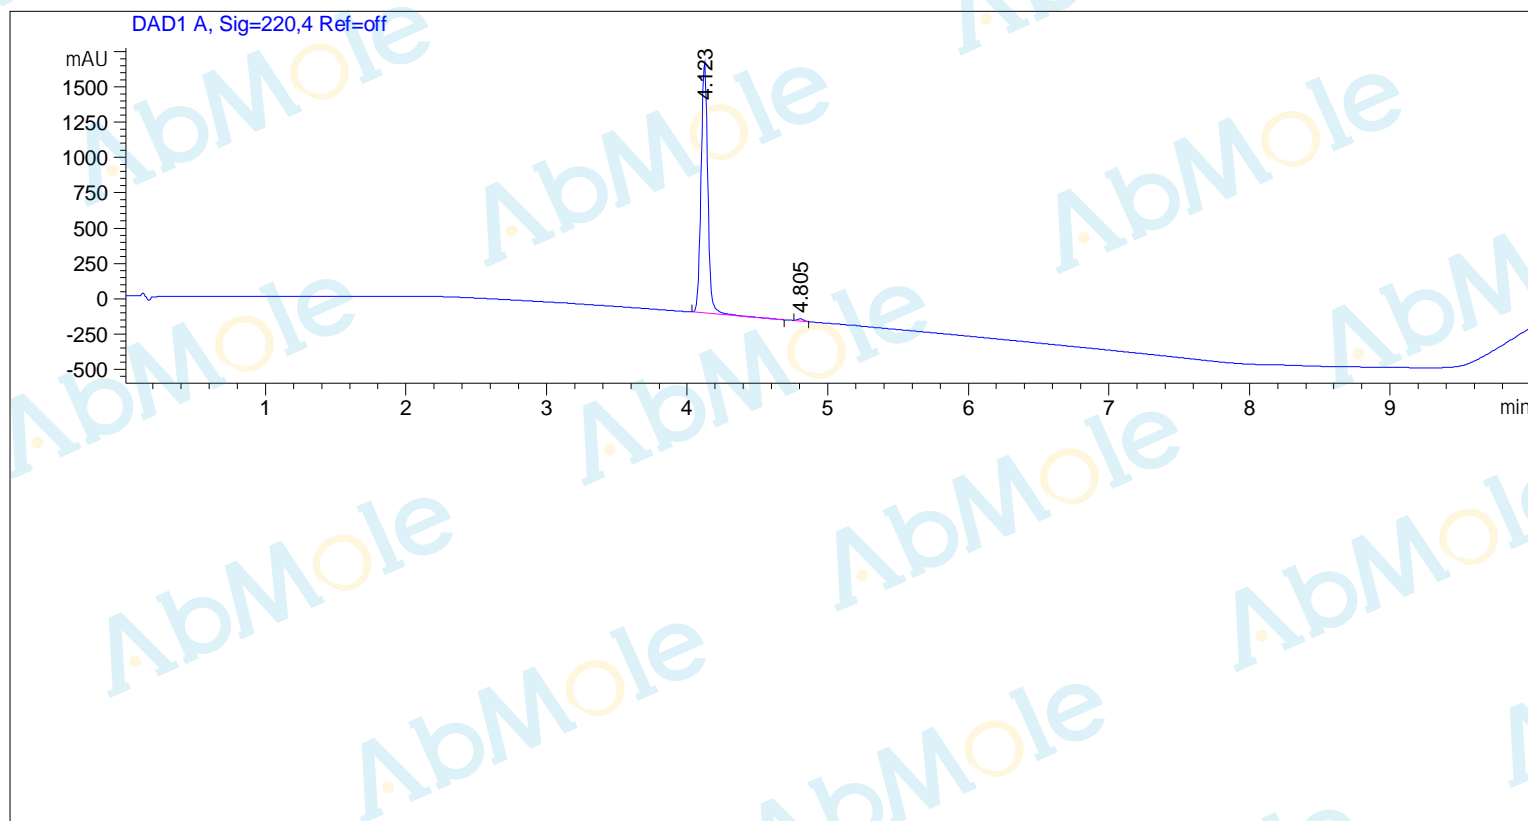

=====  
Area Percent Report  
=====

```

Sorted By      : Signal
Multiplier    : 1.0000
Dilution      : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.123	BB	0.0537	6059.09131	1782.46826	98.8209
2	4.805	MM	0.0622	72.29672	19.36433	1.1791

Totals :

6131.38803 1801.83259