


=====
Acq. Operator : admin
Sample Operator : 1
Acq. Instrument : 3 Location : P1-E-03
Sample Name : M28898-SIRT7 inhibitor 97491-01 Inj : 1
Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl

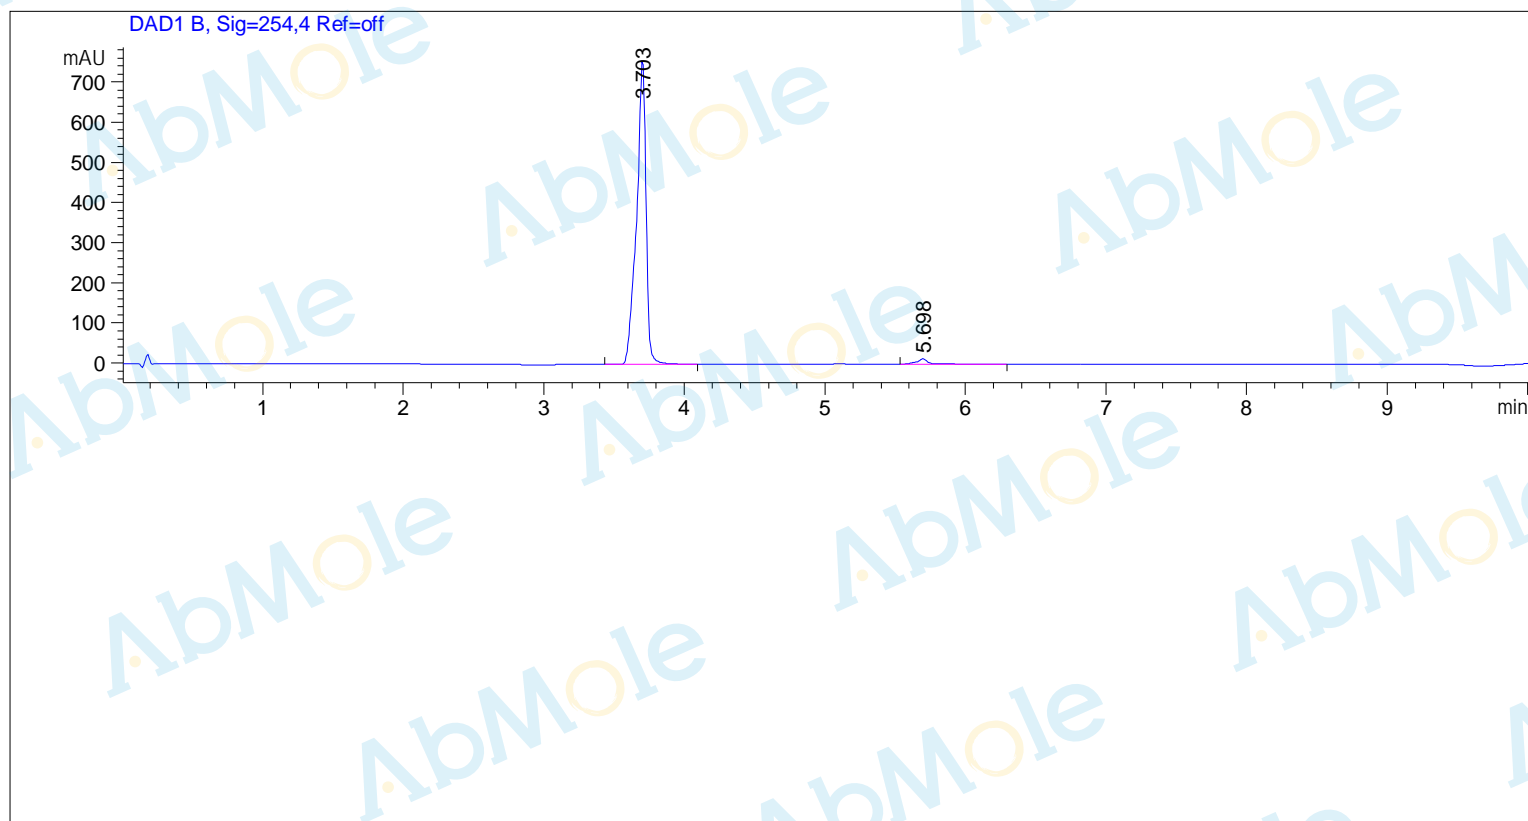

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.703	BB	0.0689	3561.16699	756.26550	98.2126
2	5.698	BB	0.0669	64.81073	13.83373	1.7874

Totals : 3636.95778 770.09923