


=====
Acq. Operator : admin
Sample Operator : M29388-VB124-01
Acq. Instrument : 3

Location : P1-A-07
Inj : 1
Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

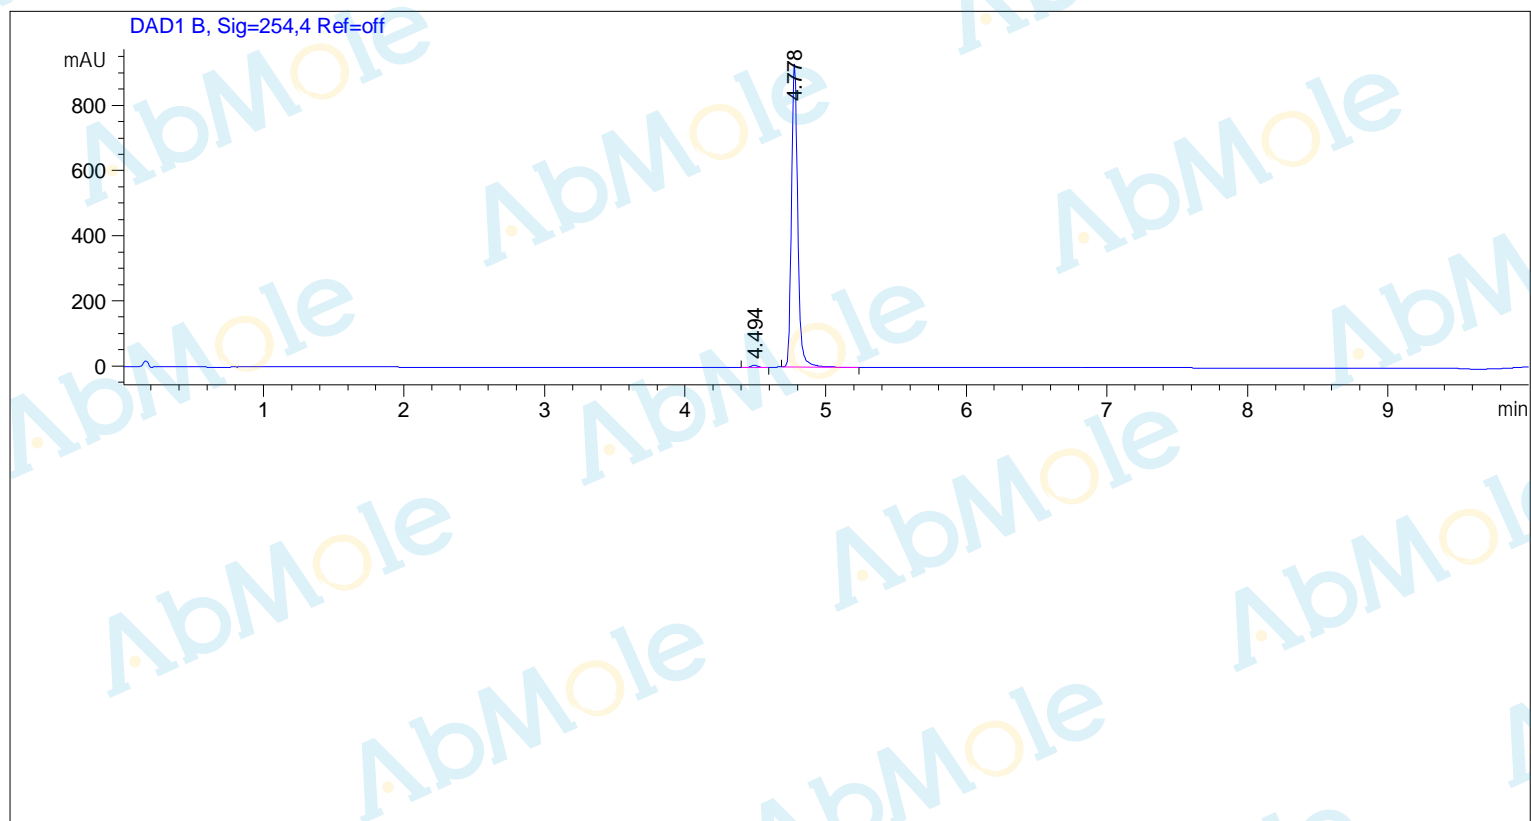

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.494	BB	0.0469	20.23906	6.76713	0.6838
2	4.778	BB	0.0488	2939.33960	930.66260	99.3162

Totals : 2959.57866 937.42973