


```

=====
Acq. Operator   : System                      Seq. Line :    3
Acq. Instrument : LC1260                     Location  : Vial 45
Injection Date  : 8/15/2022 2:10:47 PM      Inj       :    1
                                                Inj Volume: 0 µl
Different Inj Volume from Sequence ! Actual Inj Volume : 2 µl
Acq. Method     : E:\DATA\Data\20220614\20130913-01 2022-08-15 13-23-39\10-80AD 15MIN.M
Last changed    : 8/15/2022 1:23:39 PM by System
Analysis Method : D:\PUBLIC\METHOD\5-95 6MIN.M
Last changed    : 8/15/2022 4:22:05 PM
                (modified after loading)
=====
  
```

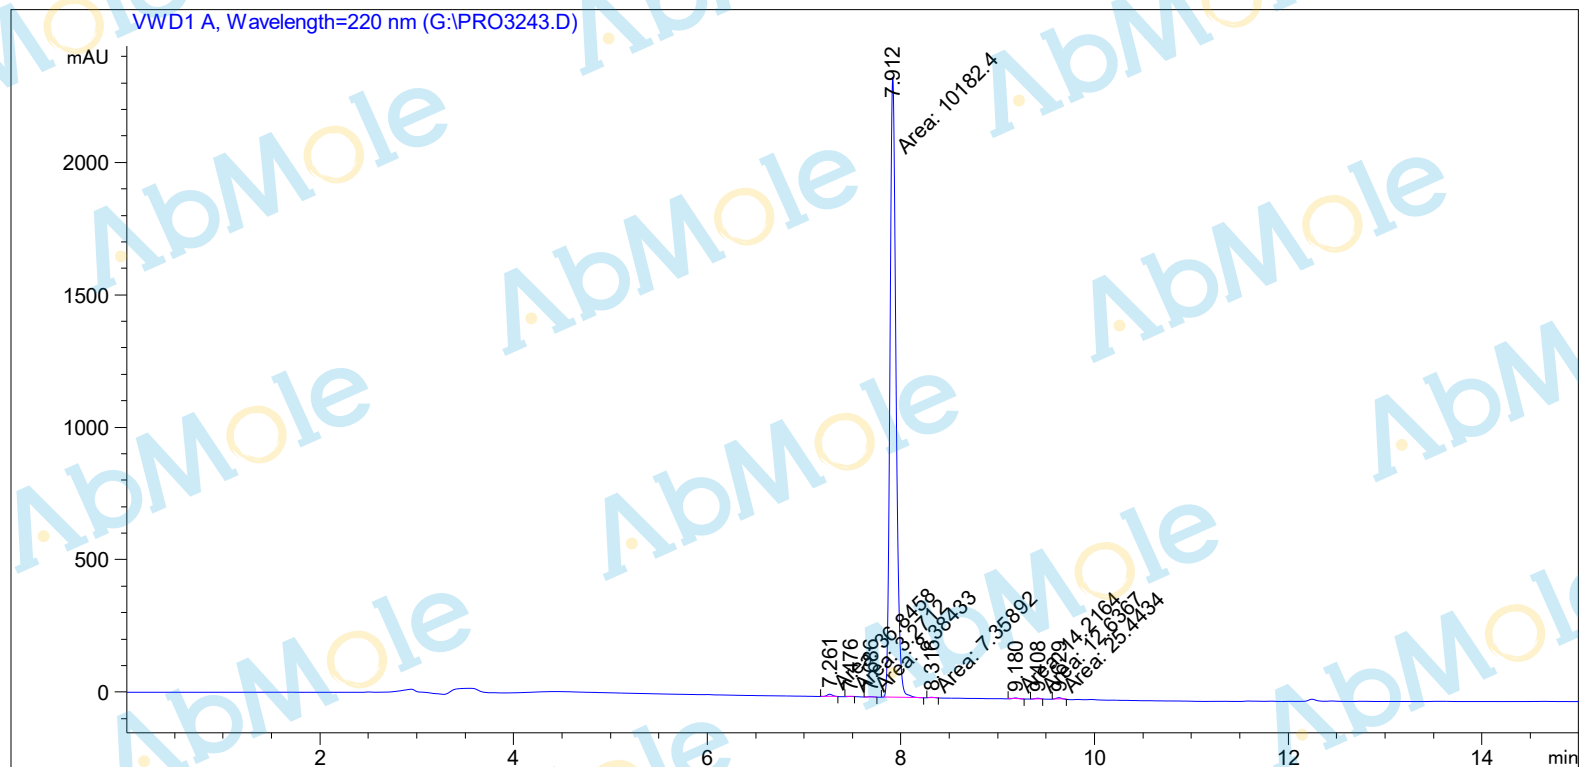

=====
 Area Percent Report
 =====

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: VWD1 A, Wavelength=220 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	7.261	MM	0.0692	36.84578	8.86969	0.3581
2	7.476	MM	0.0532	3.27120	1.02531	0.0318
3	7.686	MM	0.0711	8.38433	1.96672	0.0815

Sample Name: M3032-Static-01

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
4	7.912	MM	0.0724	1.01824e4	2343.40259	98.9490
5	8.316	MM	0.0630	7.35892	1.94823	0.0715
6	9.180	MM	0.0664	14.21642	3.56591	0.1382
7	9.408	MM	0.0619	12.63667	3.40122	0.1228
8	9.629	MM	0.0698	25.44343	6.07526	0.2473

Totals : 1.02906e4 2370.25495

*** End of Report ***