


```

=====
Acq. Operator   : admin
Sample Operator : 1
Acq. Instrument : 3
Sample Name     : M30412-NNK-01
Location       : P1-E-04
Inj            : 1
Inj Volume     : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl
=====

```

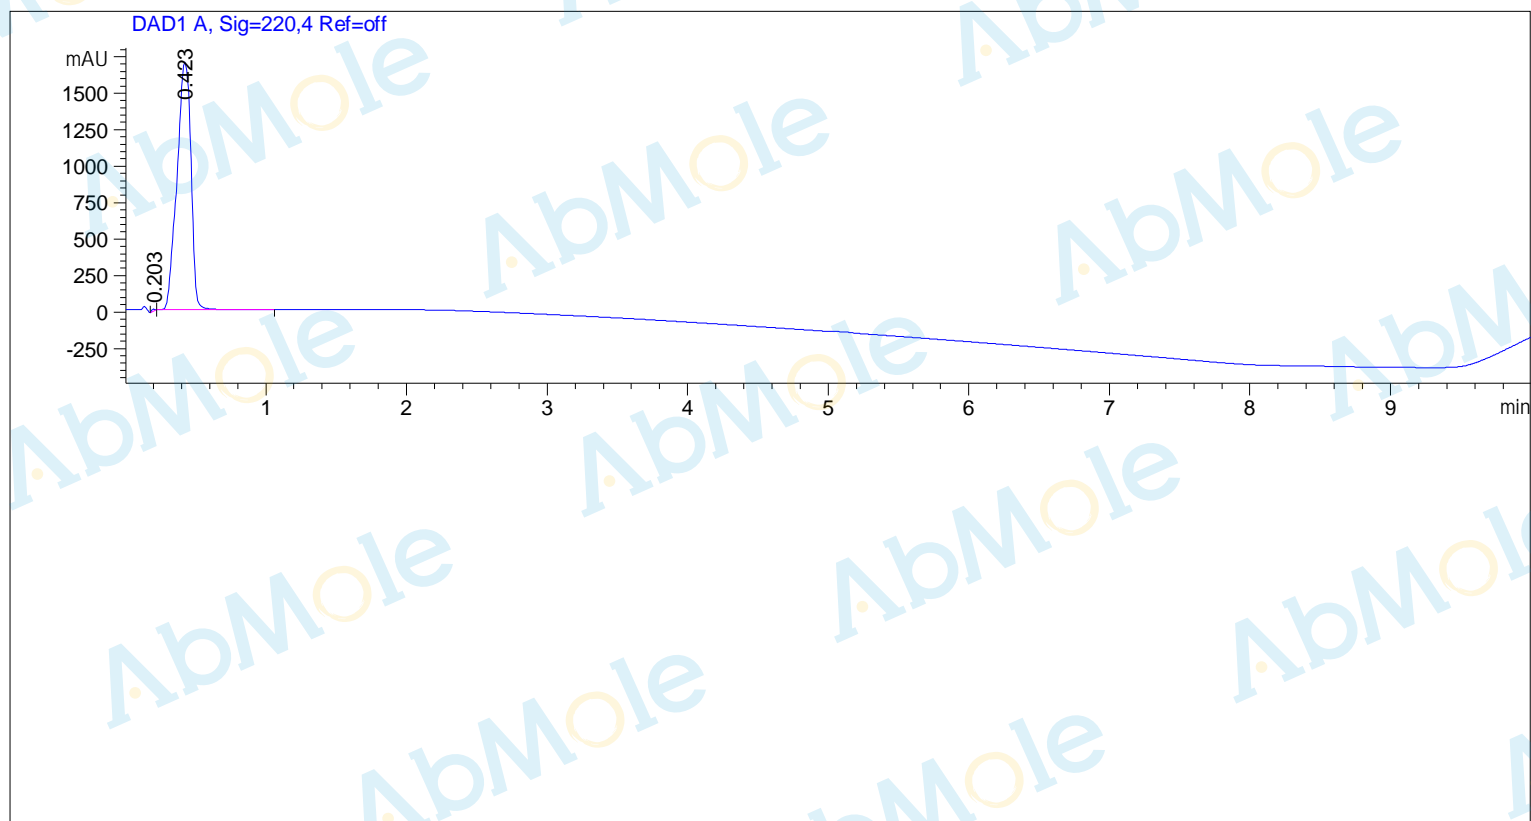

```

=====
                          Area Percent Report
=====

```

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.203	BB	0.0262	19.32076	12.40061	0.1637
2	0.423	BB	0.1072	1.17848e4	1694.03101	99.8363

Totals :

1.18041e4 1706.43162