




Sample name: M3949-AF 353-01
Instrument: A010
Inj. volume: 1
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

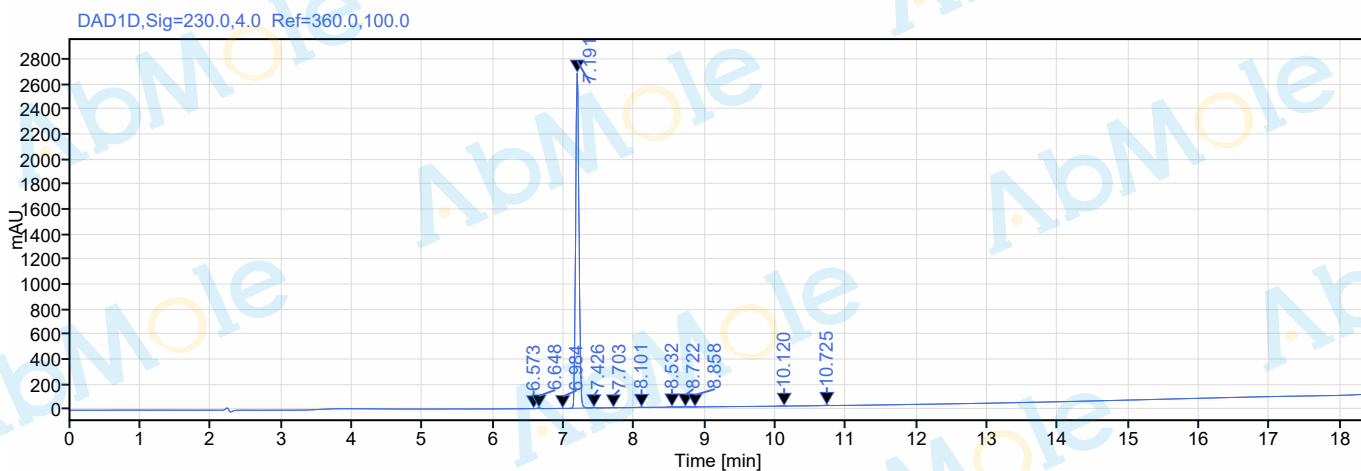

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
6.573	MM m	0.06	0.64	0.26	0.01
6.648	BB	0.12	18.56	6.47	0.21
6.984	MM m	0.16	2.85	0.48	0.03
7.191	BB	0.29	8946.05	2676.40	99.01
7.426	BB	0.18	11.43	3.49	0.13
7.703	MB m	0.13	4.41	0.99	0.05
8.101	MB m	0.14	10.02	2.81	0.11
8.532	MB m	0.14	10.59	3.04	0.12
8.722	BB	0.21	9.81	1.70	0.11
8.858	MM m	0.09	0.66	0.25	0.01
10.120	MM m	0.13	1.75	0.40	0.02
10.725	MM m	0.23	18.33	3.83	0.20