



Sample name: M45387-VBIT-4-01

Injection date:

Instrument: A010

Location:

Inj. volume: 2


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

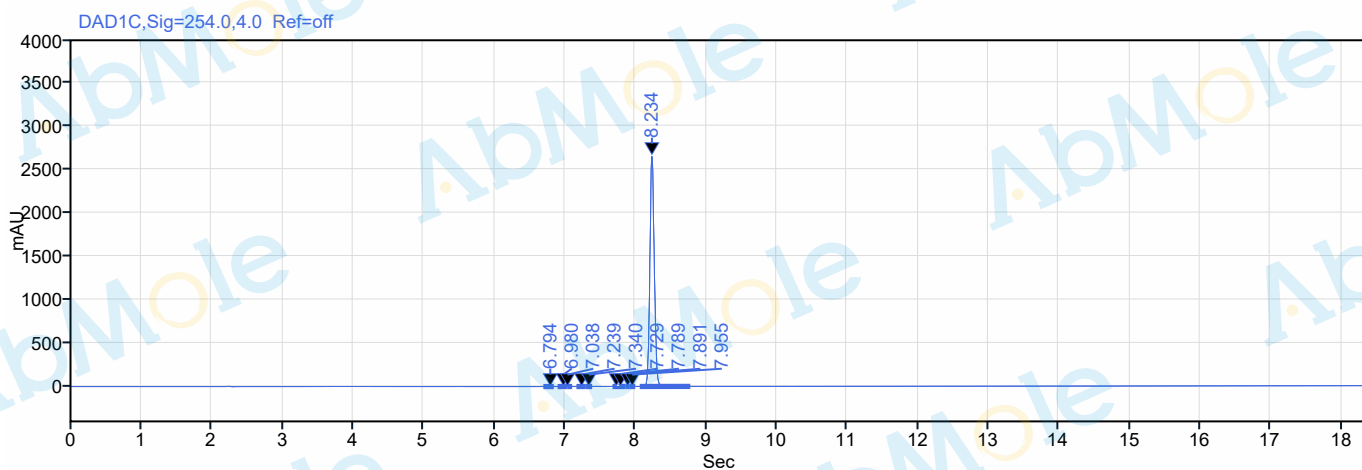

Signal: DAD1C,Sig=254.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
6.794		0.15	2.5	0.7	0.02
6.980		0.14	5.9	1.8	0.05
7.038		0.07	0.4	0.2	0.00
7.239		0.13	3.6	1.1	0.03
7.340		0.09	0.7	0.3	0.01
7.729		0.07	0.4	0.1	0.00
7.789		0.11	0.7	0.2	0.01
7.891		0.06	0.1	0.0	0.00
7.955		0.08	0.1	0.1	0.00
8.234		0.72	11646.0	2669.8	99.88