




Sample name: M5072-NS-1619-01  
Instrument: A012  
Inj. volume: 2  
Acq. method: HPLC  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

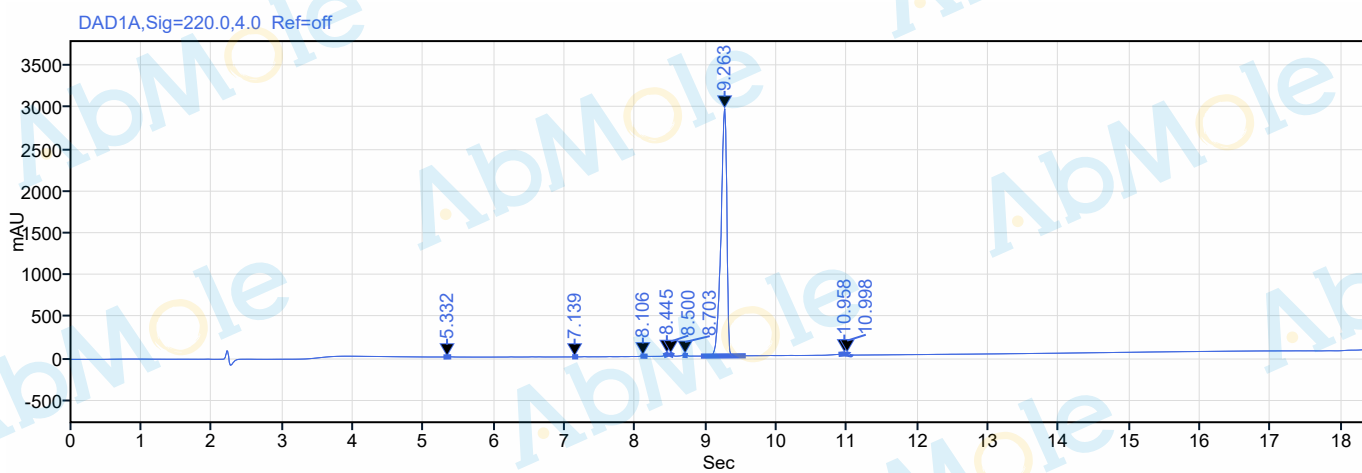

Signal: DAD1A, Sig=220.0, 4.0 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
5.332		16.4	5.1	0.094
7.139		11.1	3.9	0.064
8.106		31.6	8.9	0.182
8.445		47.8	19.0	0.275
8.500		31.6	13.1	0.182
8.703		46.6	18.0	0.268
9.263		17062.2	2952.6	98.245
10.958		62.8	18.4	0.362
10.998		56.8	18.6	0.327