




Sample name: M5145-Anisomycin-03
Instrument: A010
Inj. volume: 3
Acq. method: HPLC
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

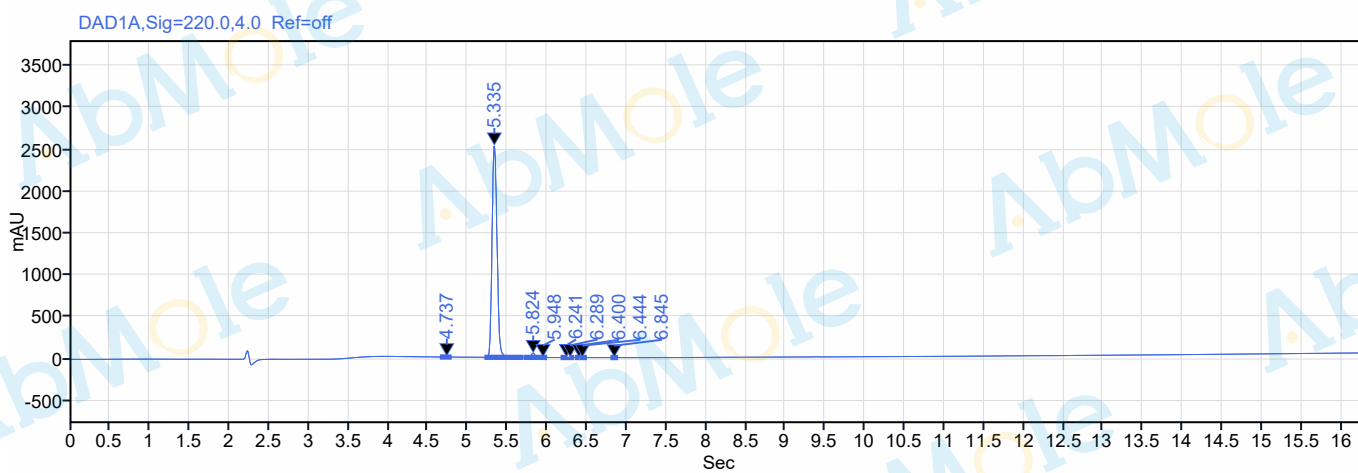

Signal: DAD1A, Sig=220.0,4.0 Ref=off

RT [min]	Peak	Area	Height	Area%
4.737		23.7	7.1	0.210
5.335		11082.7	2526.2	98.151
5.824		159.7	49.7	1.414
5.948		3.3	1.2	0.030
6.241		11.5	3.7	0.102
6.289		7.5	2.8	0.066
6.400		0.3	0.2	0.003
6.444		1.4	0.4	0.012
6.845		1.3	0.5	0.012