




Sample name: M5305-RO-3306-02  
Instrument: A010  
Inj. volume: 3  
Acq. method: HPLC  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

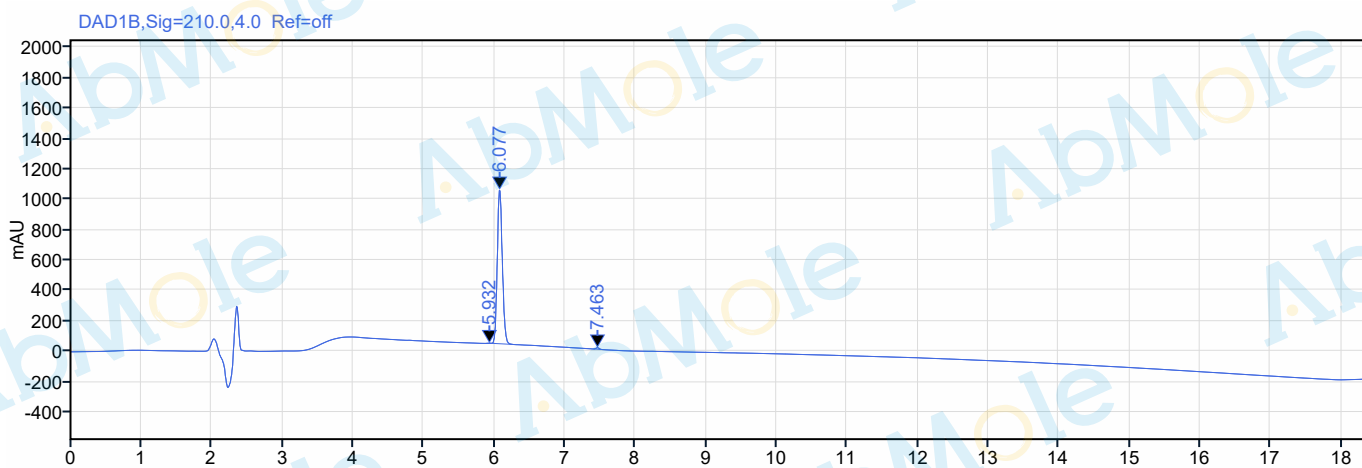

Signal: DAD1B, Sig=210.0, 4.0 Ref=off

RT [min]	Area	Height	Area%
5.932	2.58	1.11	0.05
6.077	5012.84	1012.97	99.35
7.463	30.18	9.92	0.60