


=====
Acq. Operator : admin
Sample Operator : M5650-Fluconazole-03
Acq. Instrument : 3

Location : P2-D-10

Inj : 1

Inj Volume : 0.100 µl

Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl

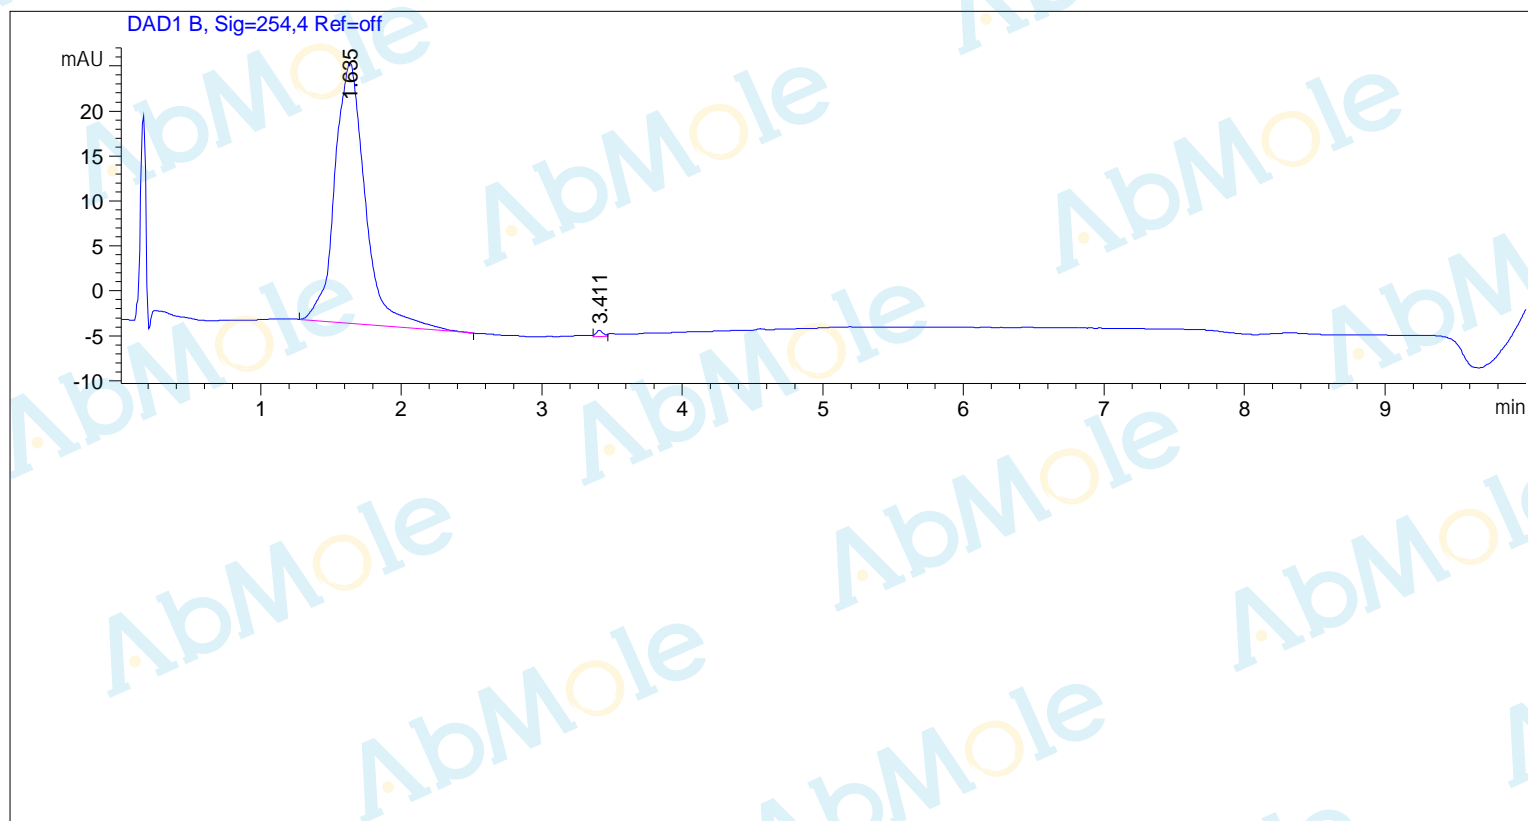

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

| Peak # | RetTime [min] | Type | Width [min] | Area [mAU*s] | Height [mAU] | Area % |
|--------|---------------|------|-------------|--------------|--------------|---------|
| 1 | 1.635 | BB | 0.2101 | 437.32416 | 28.96656 | 99.4504 |
| 2 | 3.411 | MM | 0.0606 | 2.41661 | 6.65014e-1 | 0.5496 |

Totals : 439.74077 29.63158