




Sample name: M5791-Mitomycin C-09  
Instrument: A010  
Inj. volume: 2  
Acq. method: HPLC  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

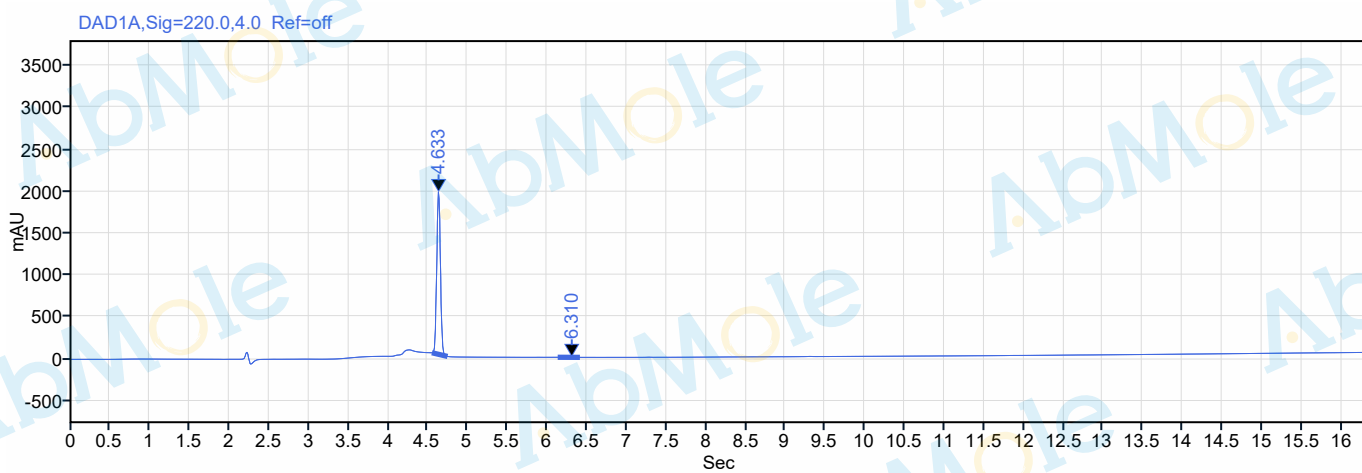

Signal: DAD1A, Sig=220.0, 4.0 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
4.633		6257.5	1935.4	99.519
6.310		30.3	3.3	0.481