
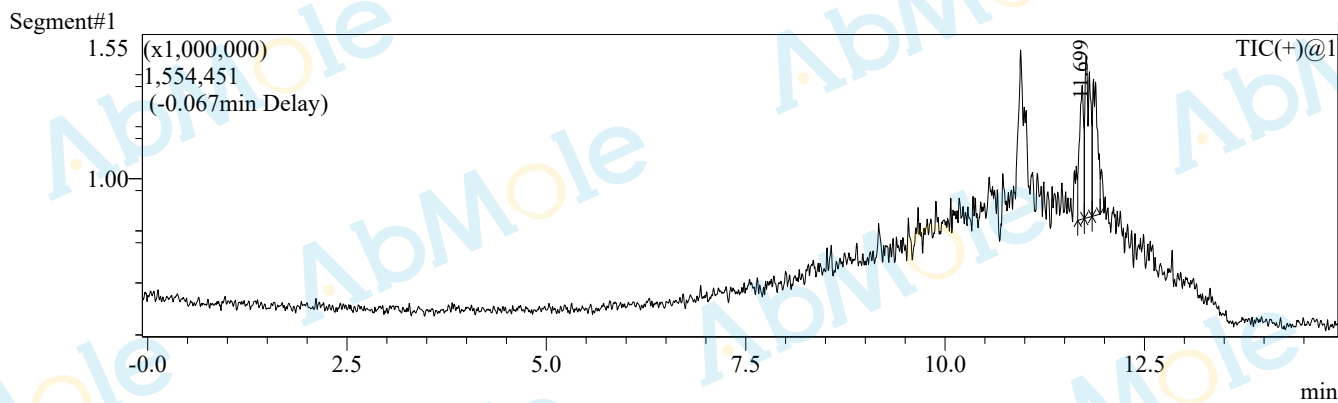
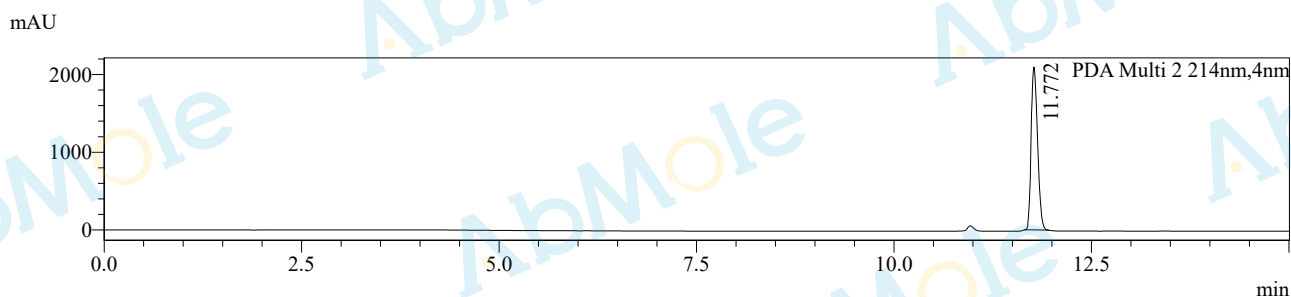


HPLC Report

Sample Name : M5855-Rilapladib-01
Method File : 5%-95%-15min
Method info. : XBridge C18 150*4.6mm 5um 1.00ml/min Column Temperature: 40 °C
Gradient: 10% B hold for 1.8 min , increase to 95 % B within 10.2 min, hold at 95 % B for 3.0 min, then back to 10% B within 0.01 min
Pump A : 0.05% NH3.H2O in H2O
Pump B : ACN

Chromatogram

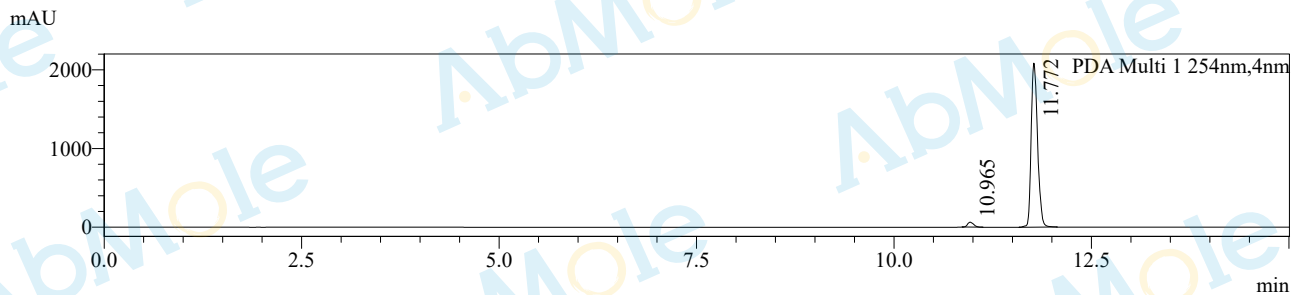

Integration Results for DAD

PDA Ch1 254nm

Peak#	Ret. Time	Height	Area	Area%
1	10.965	63101	340076	2.818
2	11.772	2083763	11727650	97.182
Total		2146863	12067726	100.000

PDA Ch2 214nm

Peak#	Ret. Time	Height	Area	Area%
1	11.772	2094782	11826240	100.000
Total		2094782	11826240	100.000