


=====
Acq. Operator : admin
Sample Operator : M5922-Ranolazine-01
Acq. Instrument : 3

Location : P1-A-05
Inj : 1
Inj Volume : 0.100 µl

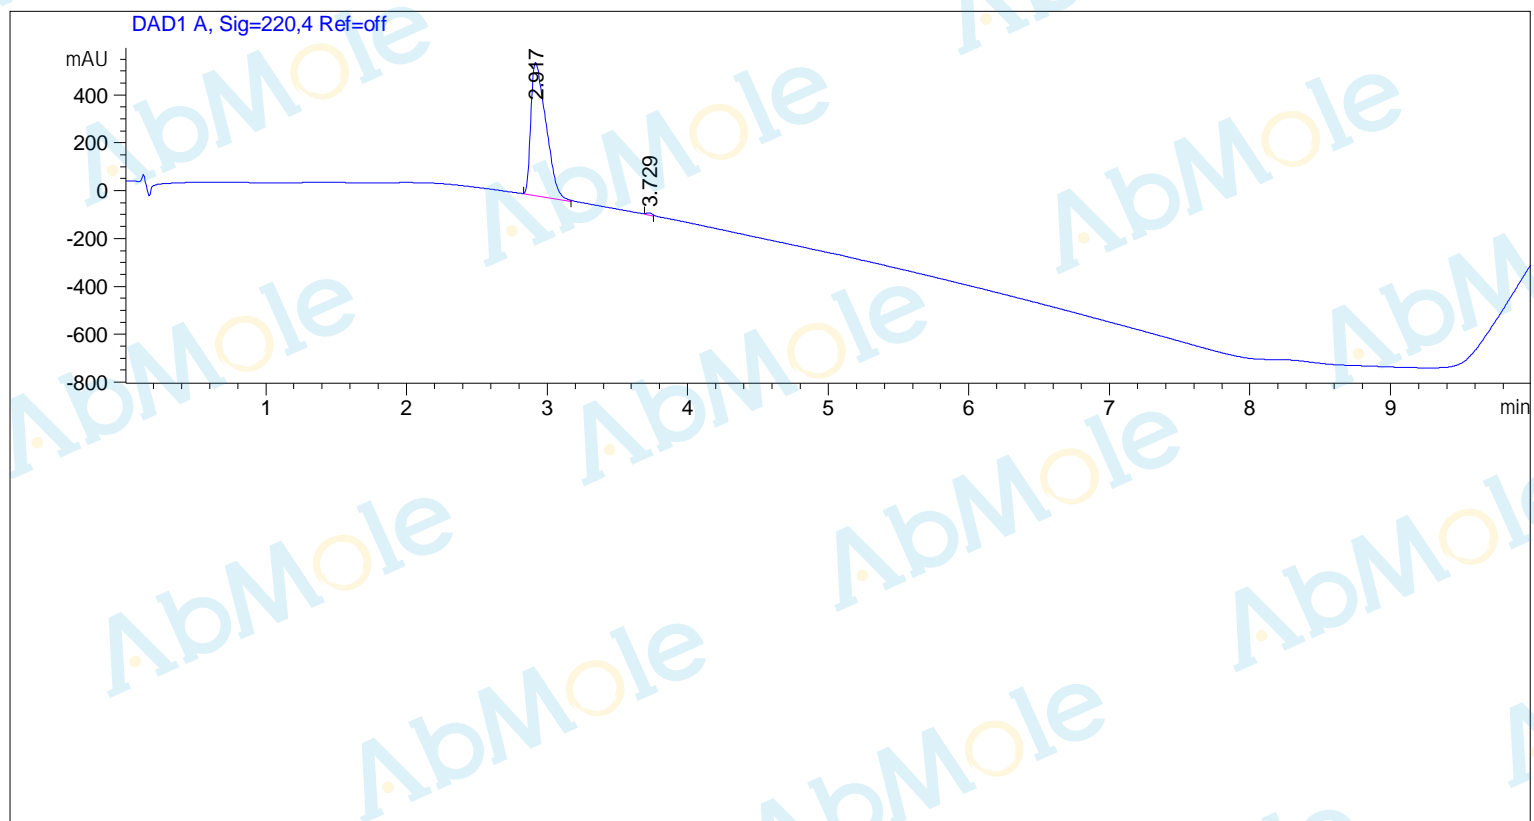

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.917	MM	0.1241	4150.63672	557.32343	99.3974
2	3.729	MM	0.0445	25.16168	9.43184	0.6026

Totals :

4175.79840 566.75527