




Agilent Technologies

Sample name: M6535-BTB-1-01
Instrument: 1.5
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

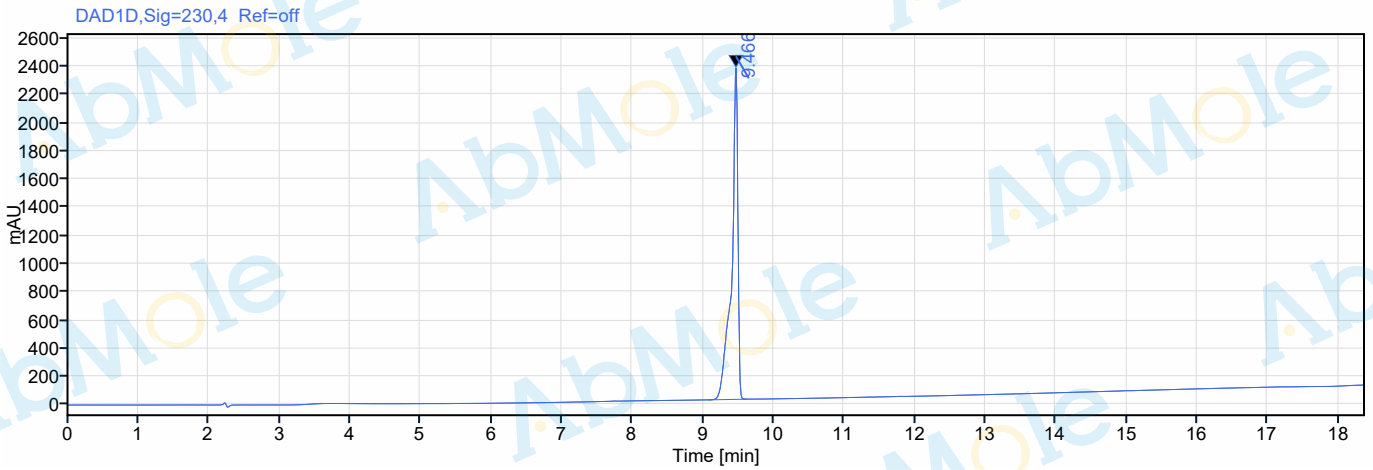

Signal: DAD1D,Sig=230,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%	Name
9.466	BV	0.54	14471.08	2350.62	100.00	
		Sum	14471.08			