




HPLC Report

Sample Name : M8994-AM095 free acid-01
Method File : B 5%-95%

Method info. : XBridge C18 150*4.6mm 5um 1.00ml/min Column Temperature: 40 °C
Gradient: 10% B hold for 1.8 min , increase to 95 % B within 10.2 min, hold at 95 % B for 3.0 min, then back to 10% B within 0.01 min

Pump A : 0.05% NH3.H2O in H2O
Pump B : ACN

Chromatogram

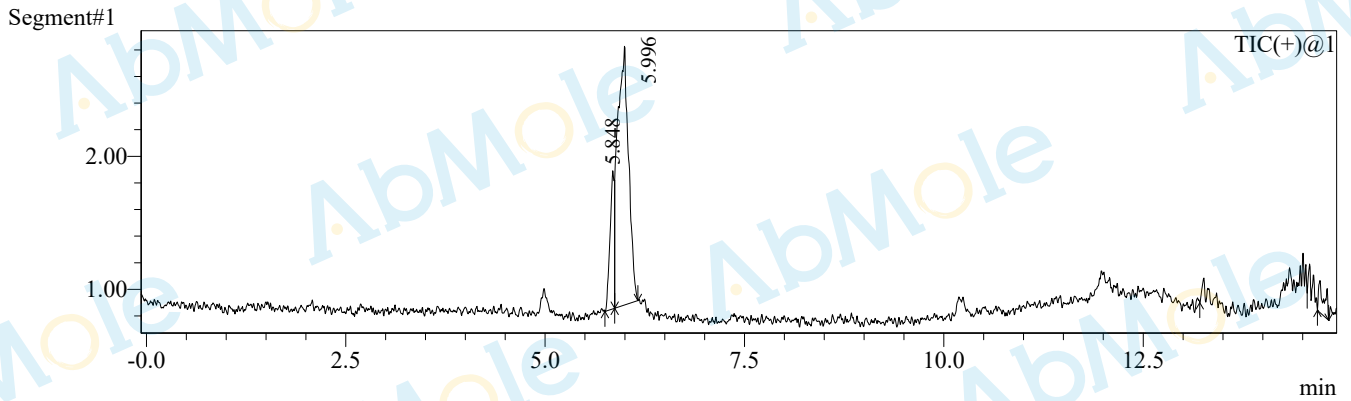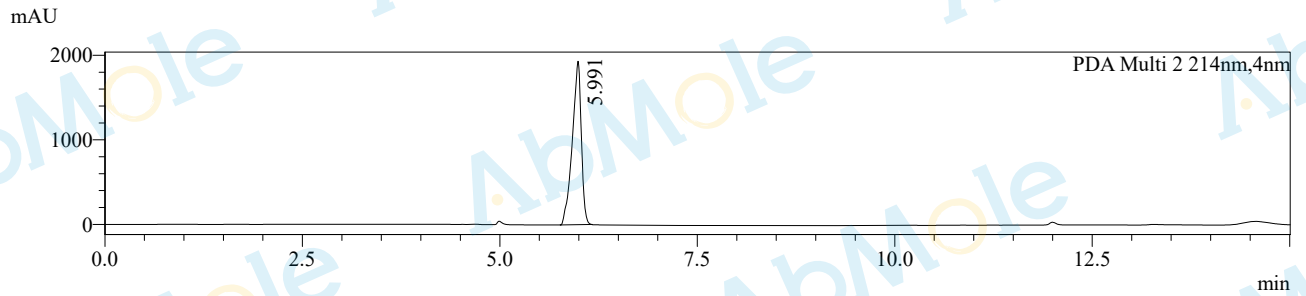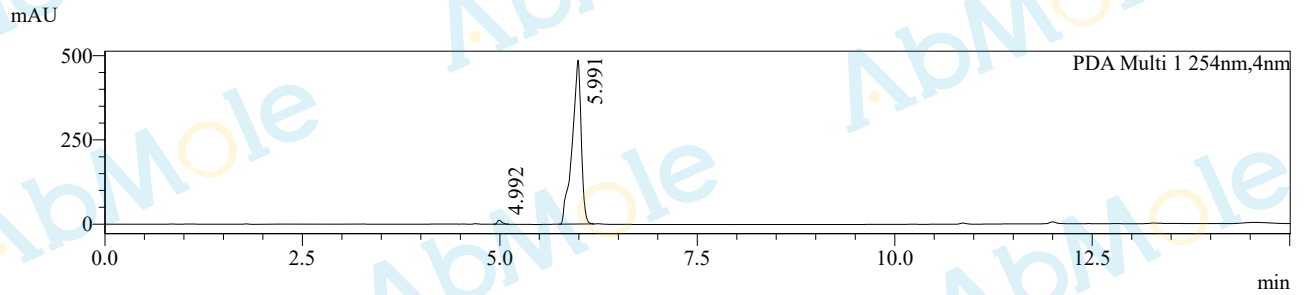

Integration Results for DAD

PDA Ch1 254nm

Peak#	Ret. Time	Height	Area	Area%
1	4.992	11484	46415	1.185
2	5.991	485598	3870963	98.815
Total		497082	3917378	100.000

PDA Ch2 214nm

Peak#	Ret. Time	Height	Area	Area%
1	5.991	1931913	15288134	100.000
Total		1931913	15288134	100.000