




Sample name: M9049-MPTP HCI-08
Instrument: 5
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

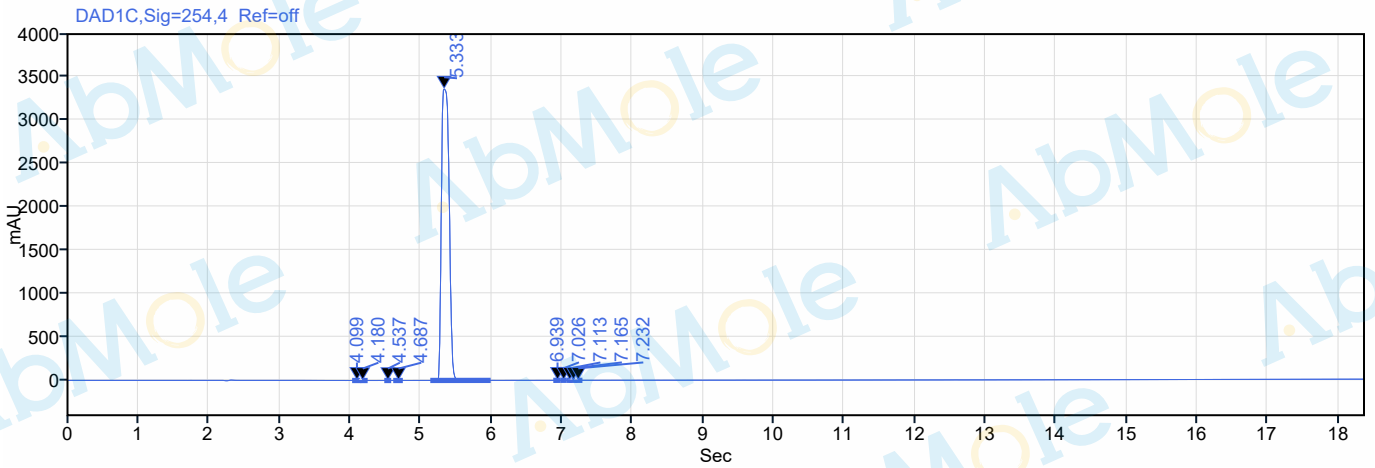

Signal: DAD1C,Sig=254,4 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
4.099		0.06	7.4	2.1	0.03
4.180		0.05	2.2	0.7	0.01
4.537		0.05	0.9	0.3	0.00
4.687		0.07	0.8	0.2	0.00
5.333		0.12	25592.1	3366.9	99.89
6.939		0.05	2.1	0.7	0.01
7.026		0.09	5.5	2.0	0.02
7.113		0.03	1.4	0.7	0.01
7.165		0.05	4.2	1.2	0.02
7.232		0.05	3.3	1.0	0.01
		Sum	25619.75		