


```

=====
Acq. Operator   : admin
Sample Operator : M9276-6-Methoxyflavanone-01
Acq. Instrument : 3
Location       : P2-E-04
Inj            : 1
Inj Volume     : 0.100 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl
=====

```

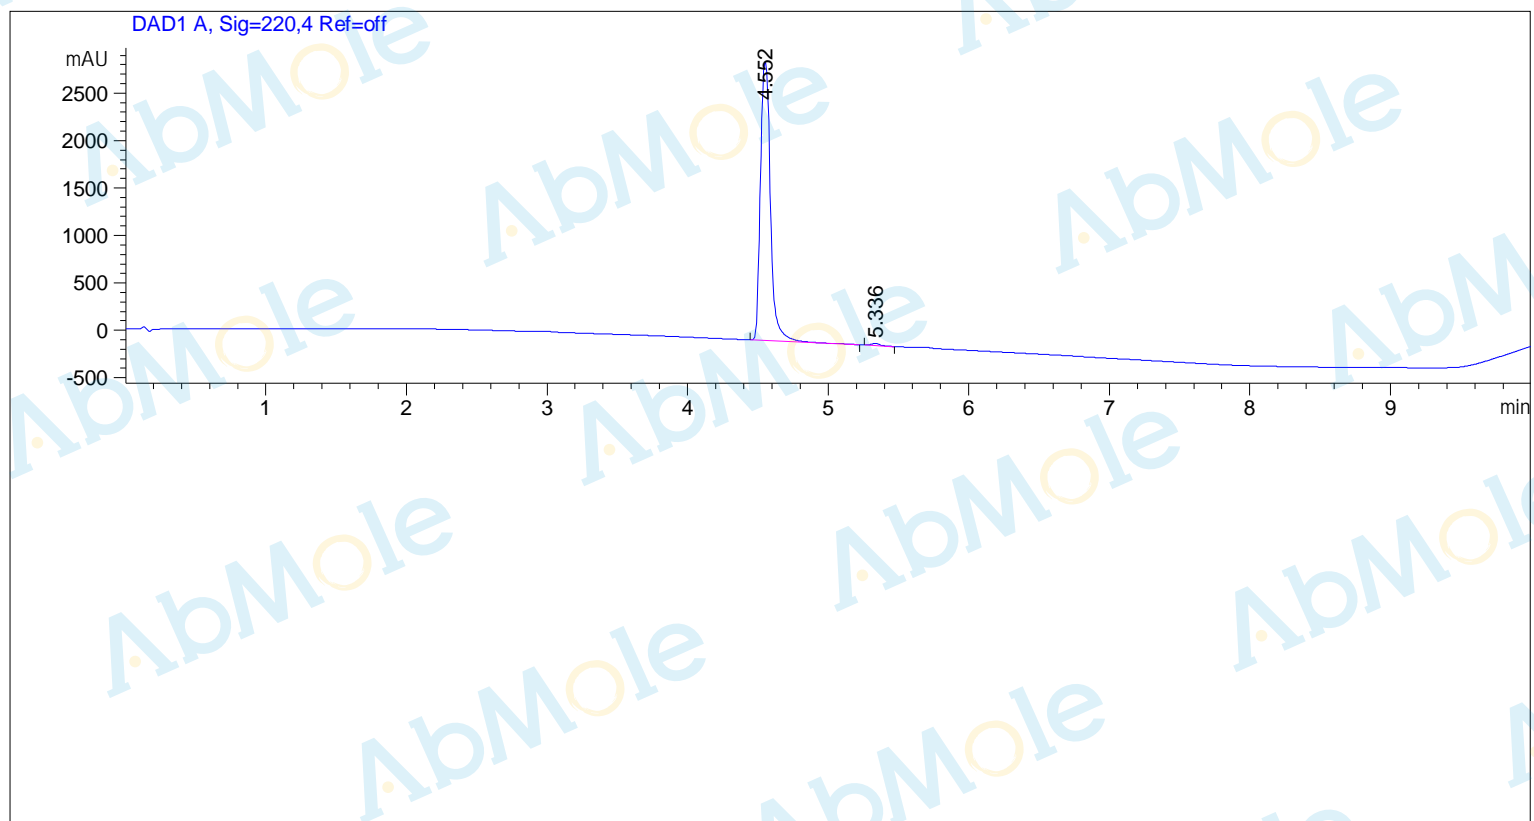

```

=====
                          Area Percent Report
=====

```

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.552	BB	0.0798	1.45640e4	2939.69751	99.3887
2	5.336	BB	0.0603	89.57745	22.56310	0.6113

Totals :

1.46535e4 2962.26061