




Sample name: M9378-NHS-Biotin-02
Instrument: 5
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

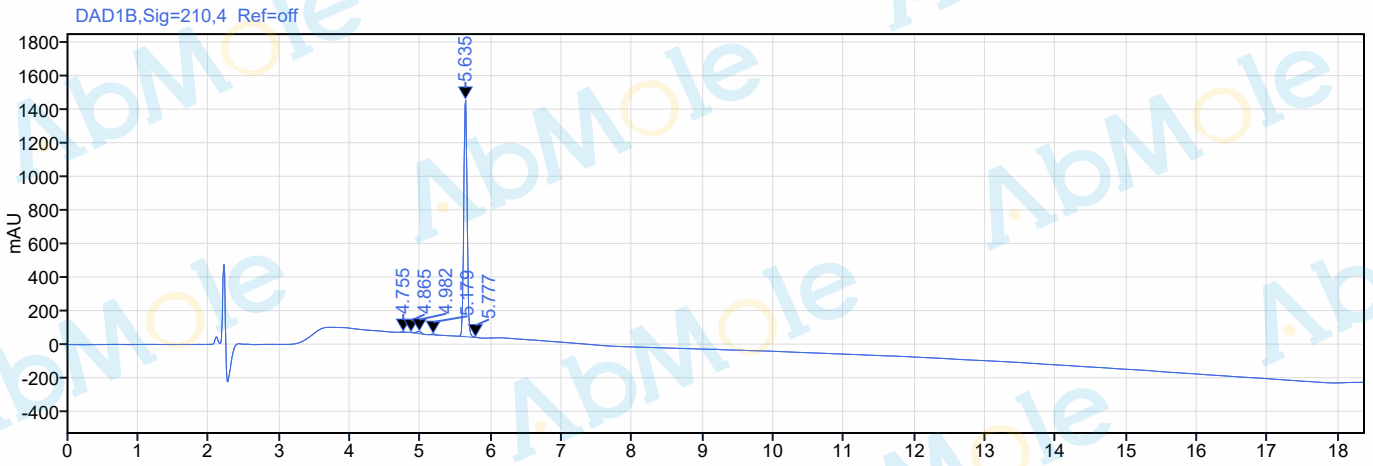

Signal: DAD1B, Sig=210,4 Ref=off

RT [min]	Area	Height	Area%
4.755	5.23	2.06	0.11
4.865	4.54	1.94	0.09
4.982	54.64	12.35	1.13
5.179	19.17	5.61	0.40
5.635	4730.69	1411.58	98.18
5.777	3.97	1.43	0.08