




HPLC Report

Sample Name :M9735-ND-646-01
Method File :B 5%-95%-15min-P.lcm

Method info. : XBridge C18 150*4.6mm 5um 1.00ml/min Column Temperature: 40 °C
Gradient: 10% B hold for 1.8 min , increase to 95 % B within 10.2 min, hold at 95 % B for 3.0 min, then back to 10% B within 0.01 min

Pump A : 0.05% NH3.H2O in H2O
Pump B : ACN

Chromatogram

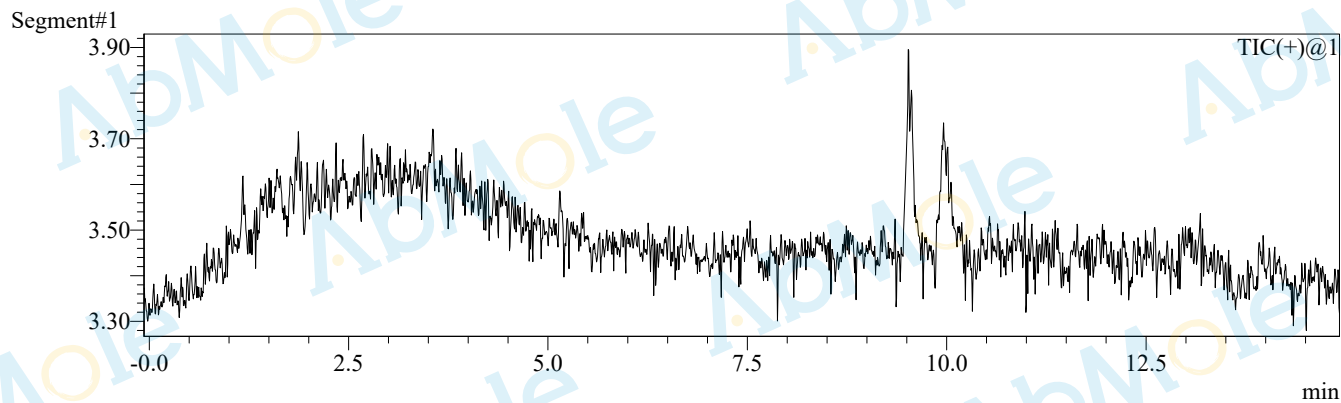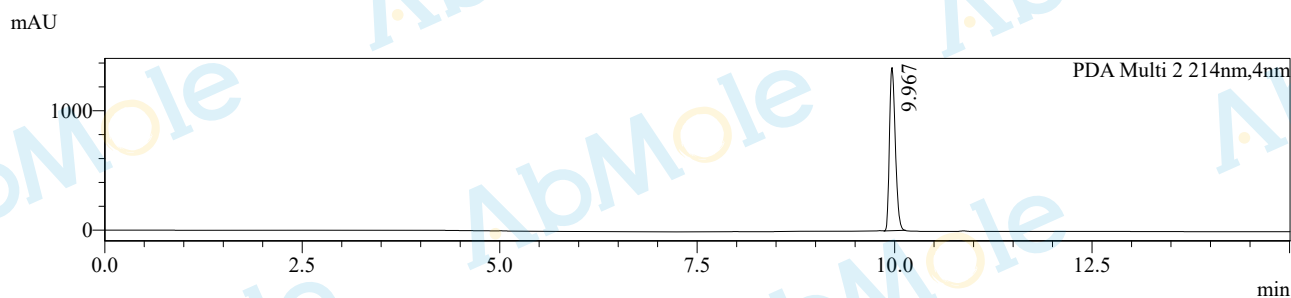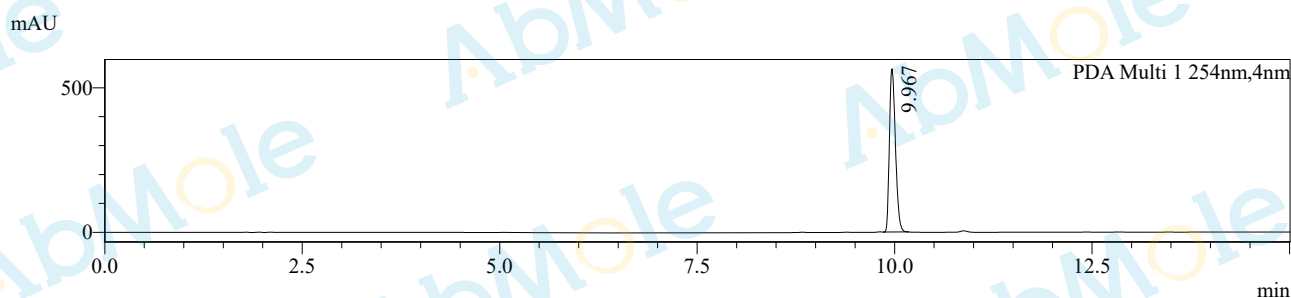

Integration Results for DAD

PDA Ch1 254nm

Peak#	Ret. Time	Height	Area	Area%
1	9.967	564939	2996368	100.000
Total		564939	2996368	100.000

PDA Ch2 214nm

Peak#	Ret. Time	Height	Area	Area%
1	9.967	1366859	7032596	100.000
Total		1366859	7032596	100.000