



7.173  
7.105  
6.754  
6.733

3.329  
2.852  
2.786  
2.510

1.545  
1.276  
1.256  
0.862


0.009

Current Data Parameters  
NAME MG149-01  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20191012  
Time\_ 12.54  
INSTRUM spect  
PROBHD 5 mm PADUL 13C  
PULPROG zg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 199.46  
DW 62.400 usec  
DE 6.50 usec  
TE 0 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 400.1324710 MHz  
NUC1 1H  
P1 10.00 usec  
PLW1 20.00000000 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

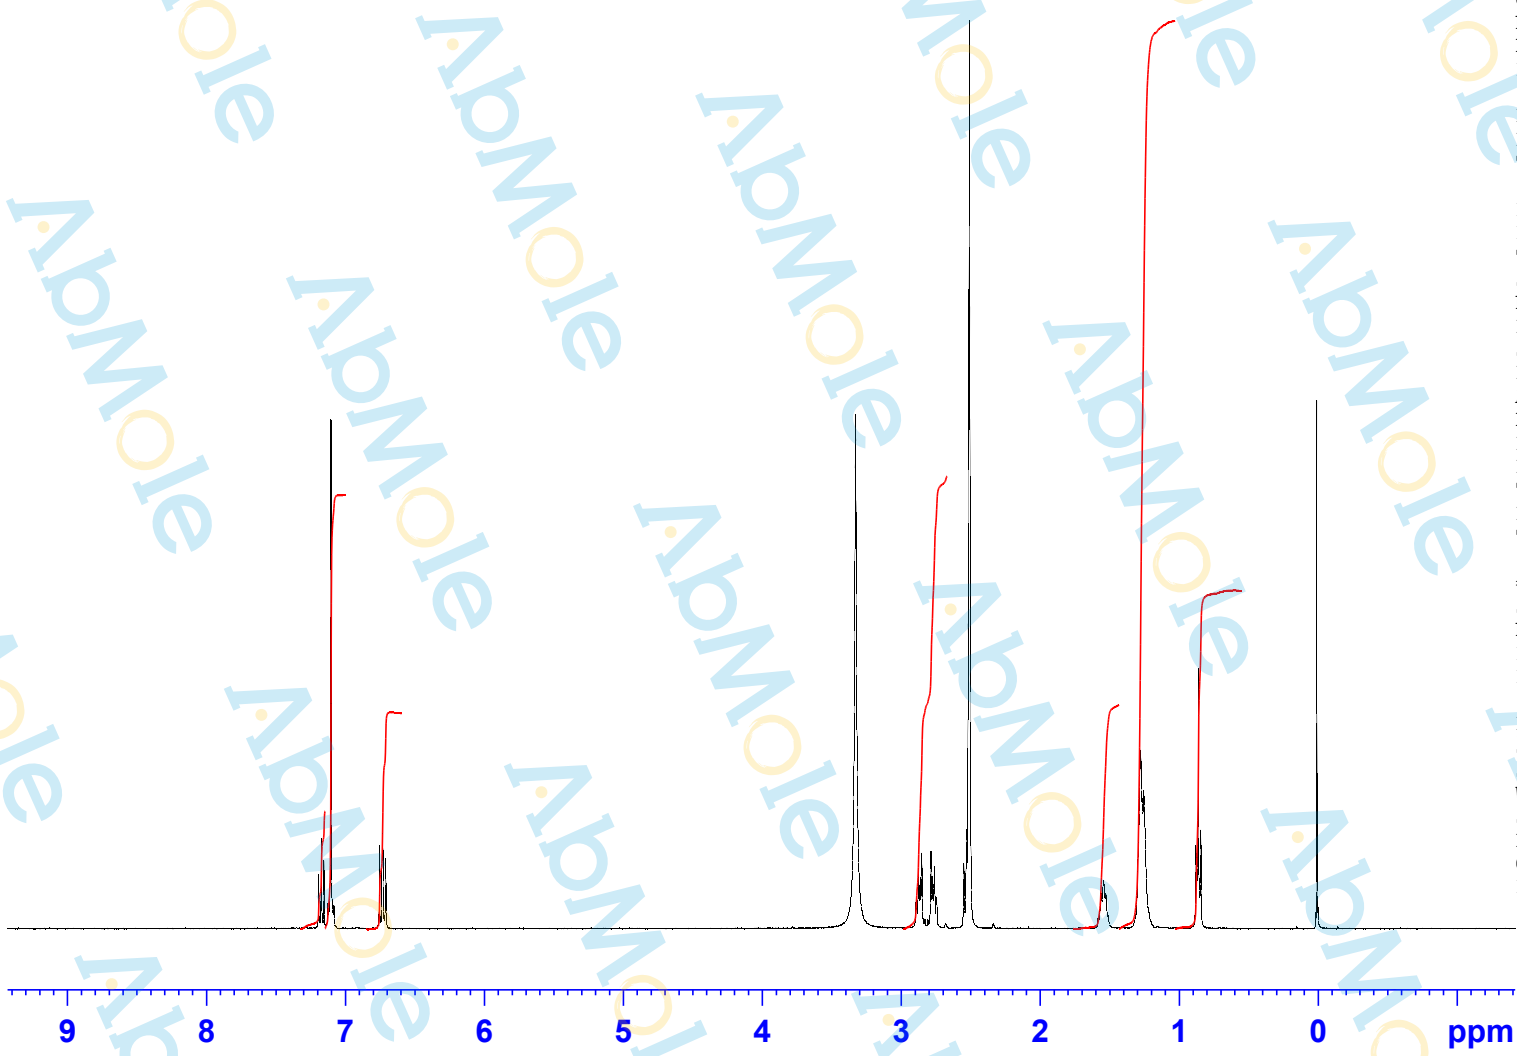

1.09  
4.02  
2.00

4.19

2.08  
8.41  
3.13

0.009