

File D:\DATA

Injection Date : 07-May-17, 20:45

Sample Name : MK-1775-01

Acq. Operator : HPLC

Spec. Reported : MS Integration

Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Sample Info :



Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B

Flow Rate: 1.2 ml/min

Column: Eclipse XDB-C18,4.6*150mm,5um

Oven Temperature: 40 C

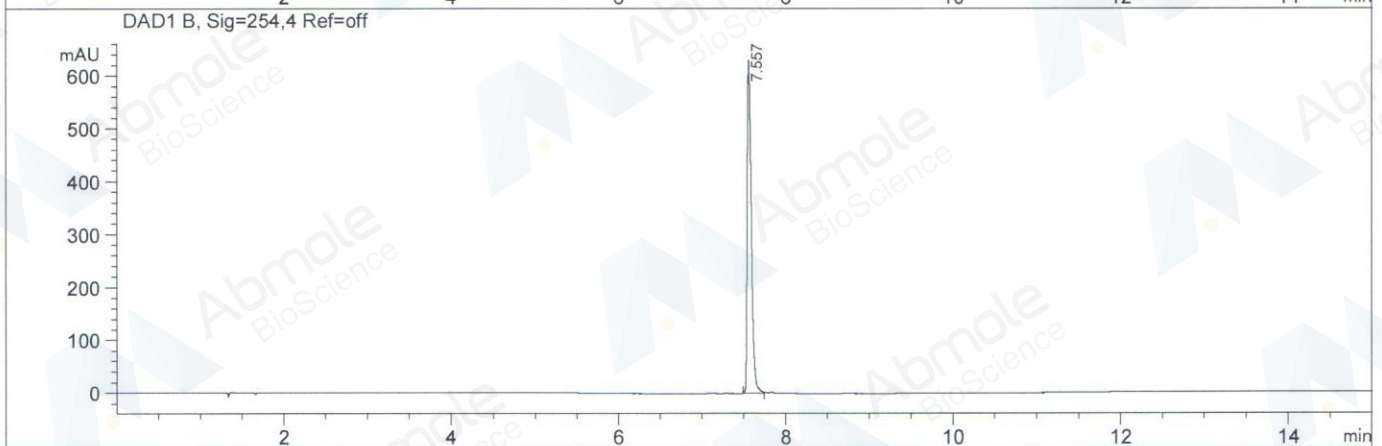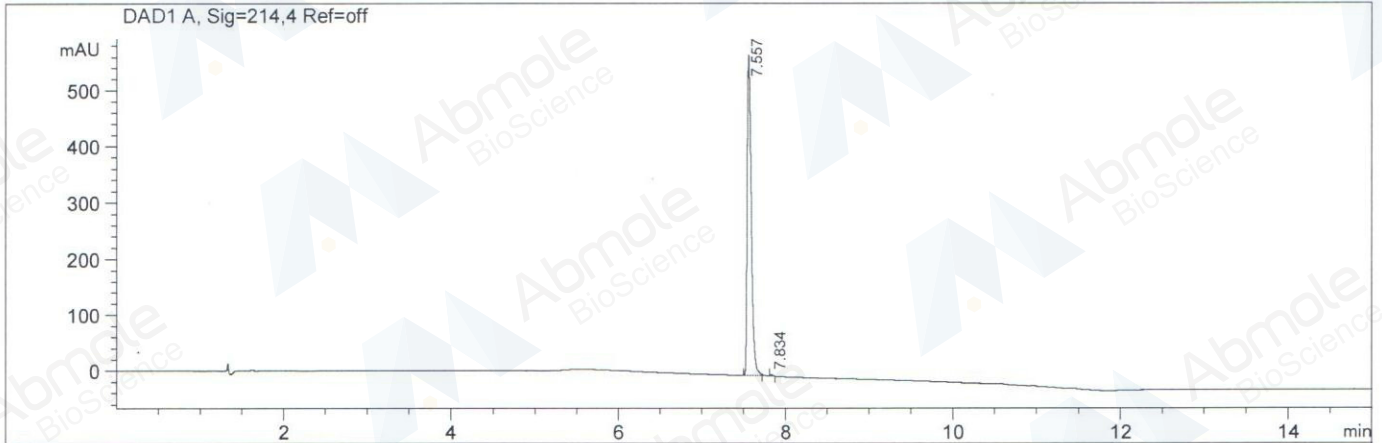

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.56	0.05	1914.86	572.13	99.79
7.83	0.03	4.09	2.20	0.21

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
7.56	0.05	2122.24	631.28	100.00