

File D:\DATA\OSI-027-HPLC

Acq. Method : D: HPLC

Analysis Method : D: HPLC

Sample Info : Easy-Access Method:

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN (0.01%TFA)

Gradient

Time 0 8 15


B % 5 95 95

Flow Rate: 1.0mL/min


Oven temperature: 40C

Column: SUNFIRE C18, 150*4.6mm, 3.5um

DAD1 A, Sig=214,4 Ref=off

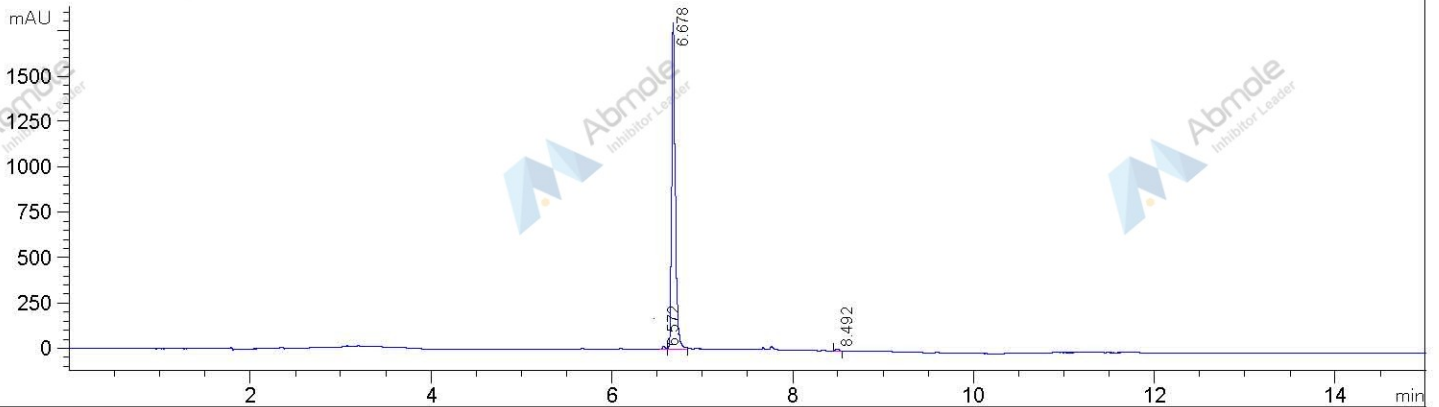

DAD1 B, Sig=254,4 Ref=off

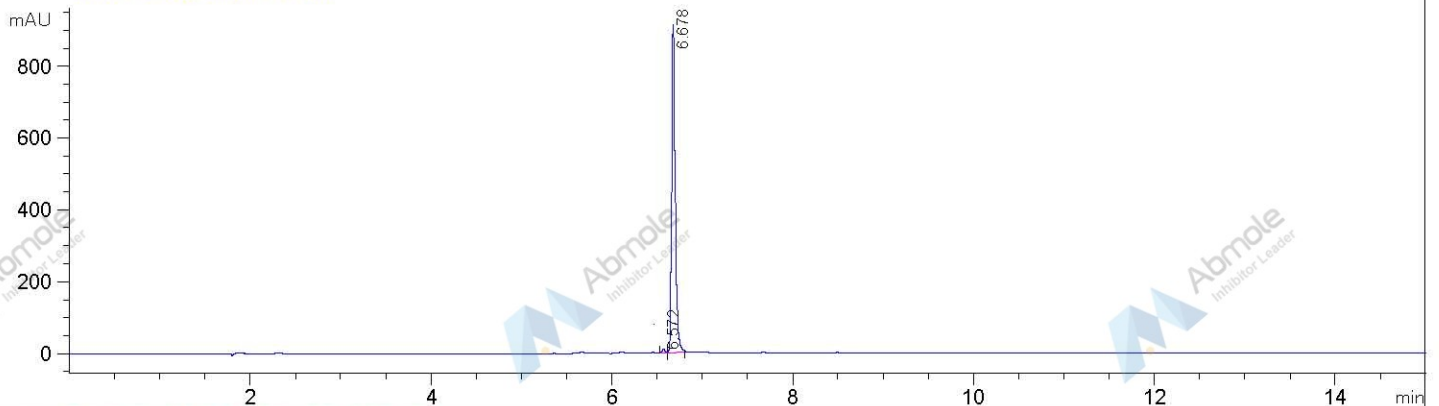

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
6.57	0.03	34.26	15.16	0.64
6.68	0.04	4975.31	1795.50	98.98
8.49	0.04	20.38	8.48	0.38

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.57	0.03	22.07	10.02	0.84
6.68	0.04	2484.18	913.39	99.16