

1. Analysis Information

Sample Name: SF 1670-01
Operator: David
Injection Date: 7/7/2020 9:55:36 AM
Batch No.: M7290-01


2. HPLC Condition

Column: Athena C18, 3 μ m, 2.1mm \times 100 mm
Solvent A: 0.1% H3PO4 in 100% Acetonitrile
Solvent B: 0.1% H3PO4 in 100% Water

Gradient:	Time	A	B
	0.0min	10%	90%
	6.0min	95%	5%
	10.0min	95%	5%
	10.0min	Stop	Stop

Flow rate: 0.5ml/min
Wavelength: 280nm
Volume: 3.0 μ l

3. Result

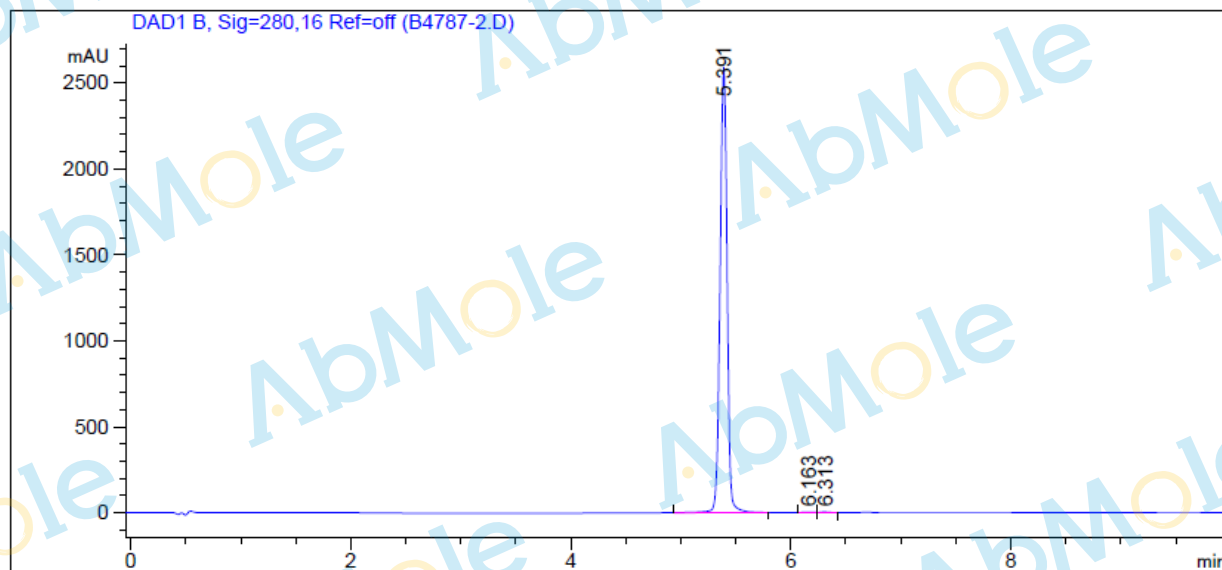

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.391	1.15297e4	99.7205
2	6.163	16.67959	0.1443
3	6.313	15.63292	0.1352