

File D:\DATA\

Injection Date : 27 Nov 16 9:45 am +0800

Tgt Mass (EZX) :

Sample Name : TG101348-01

Location : P1-C-02

Acq. Operator : LCMS

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : D:\METHODS\1-POS-3MIN.M

Analysis Method : D:\METHODS\1-POS-3MIN.M

Sample Info : *** No target masses specified ***

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5%-95% B in 1.2min


Flow Rate: 2.2 ml/min

Column: Poroshell 120 EC-C18, 4.6*30mm, 2.7um


Oven Temperature: 50 C

Mass Range: 110-1500


*ADC1 A, ELSD

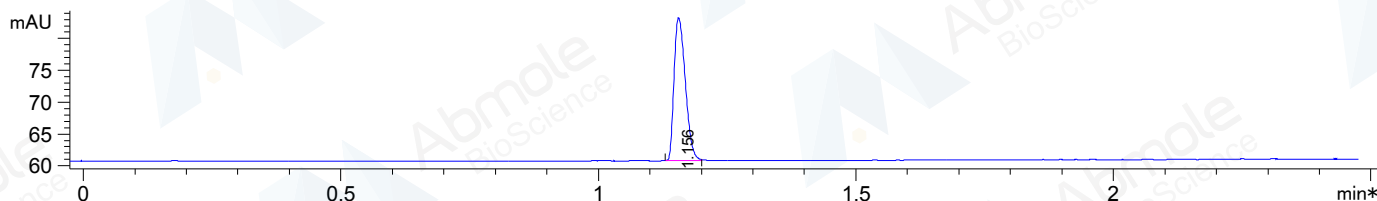


*DAD1 A, Sig=214,4 Ref=off

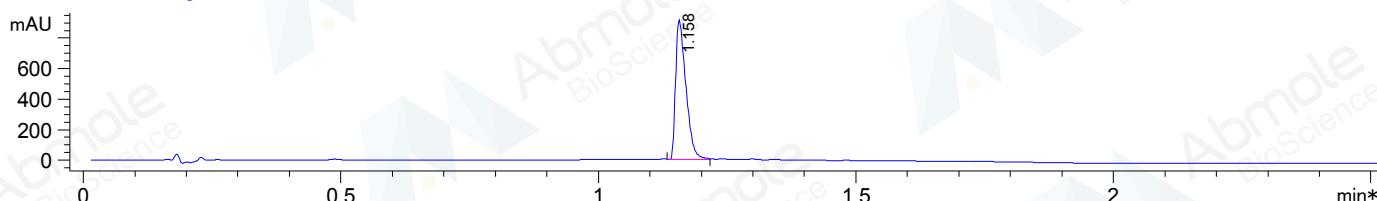

*DAD1 B, Sig=254,4 Ref=off

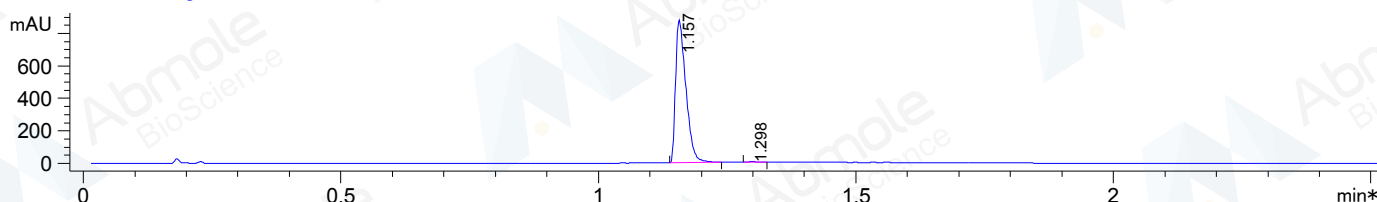

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

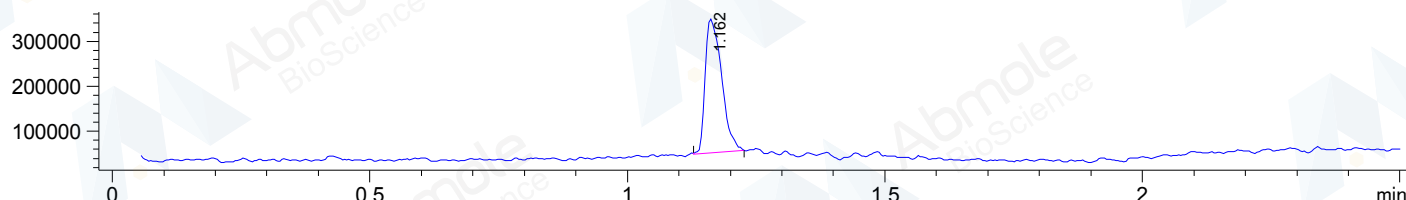

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.16	0.02	34.39	22.46	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.16	0.02	1279.42	919.24	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.16	0.02	1228.11	879.00	99.56
1.30	0.01	5.45	6.27	0.44

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

