


LC/MS Report


Injection Date : 6 Apr 21
Sample Name : Thiamine chloride-01

Method Info : Mobile Phase : A:water(0.01%TFA) B:ACN(0.01%TFA)
Gradient:5%B increase to 95%B within 1.5min,95%B for 1.5min
Flow Rate :2.0ml/min
Column :SunFire C18 3.5um, 4.6mm*50mm
Column Temperature:50C
Detection:UV(214nm,4nm) and MS(ESI,POS Mode,110-1300amu)

*DAD1 A, Sig=2144 Ref=off

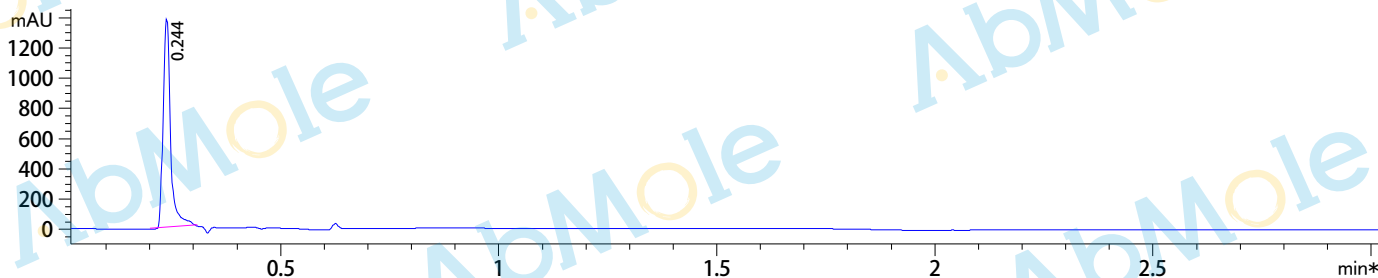

*DAD1 B, Sig=2544 Ref=off

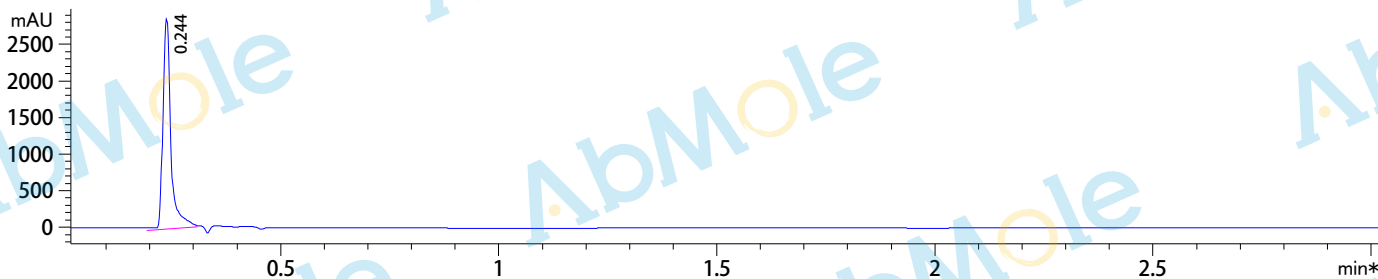

MSD1 TIC, MS File ES-AP I, Pos, Scan, Frag: 100



Integration Results for DAD1 A, Sig=2144 Ref=off

RetTim	Width	Area	Height	Area%
0.24	0.02	1241.76	1360.04	100.00

Integration Results for DAD1 B, Sig=2544 Ref=off

RetTim	Width	Area	Height	Area%
0.24	0.02	1137.84	2853.27	100.00

Ret. Time: 0.24

<<<< POSITIVE SPECTRA >>>>

