




10.332  
9.895  
8.656  
7.572  
7.556  
7.540  
7.515  
7.499  
7.496  
7.454  
7.449  
7.438  
7.433  
7.415  
7.409  
7.399  
7.391  
7.382  
7.371  
7.351  
7.332  
7.322  
7.301  
5.767  
5.182  
5.168  
5.154  
4.989  
4.497  
4.483  
3.608  
3.598  
3.551  
3.533  
3.334  
3.311  
2.514  
2.510  
2.506  
2.287  
1.942  
1.283  
1.274  
1.243  
0.008

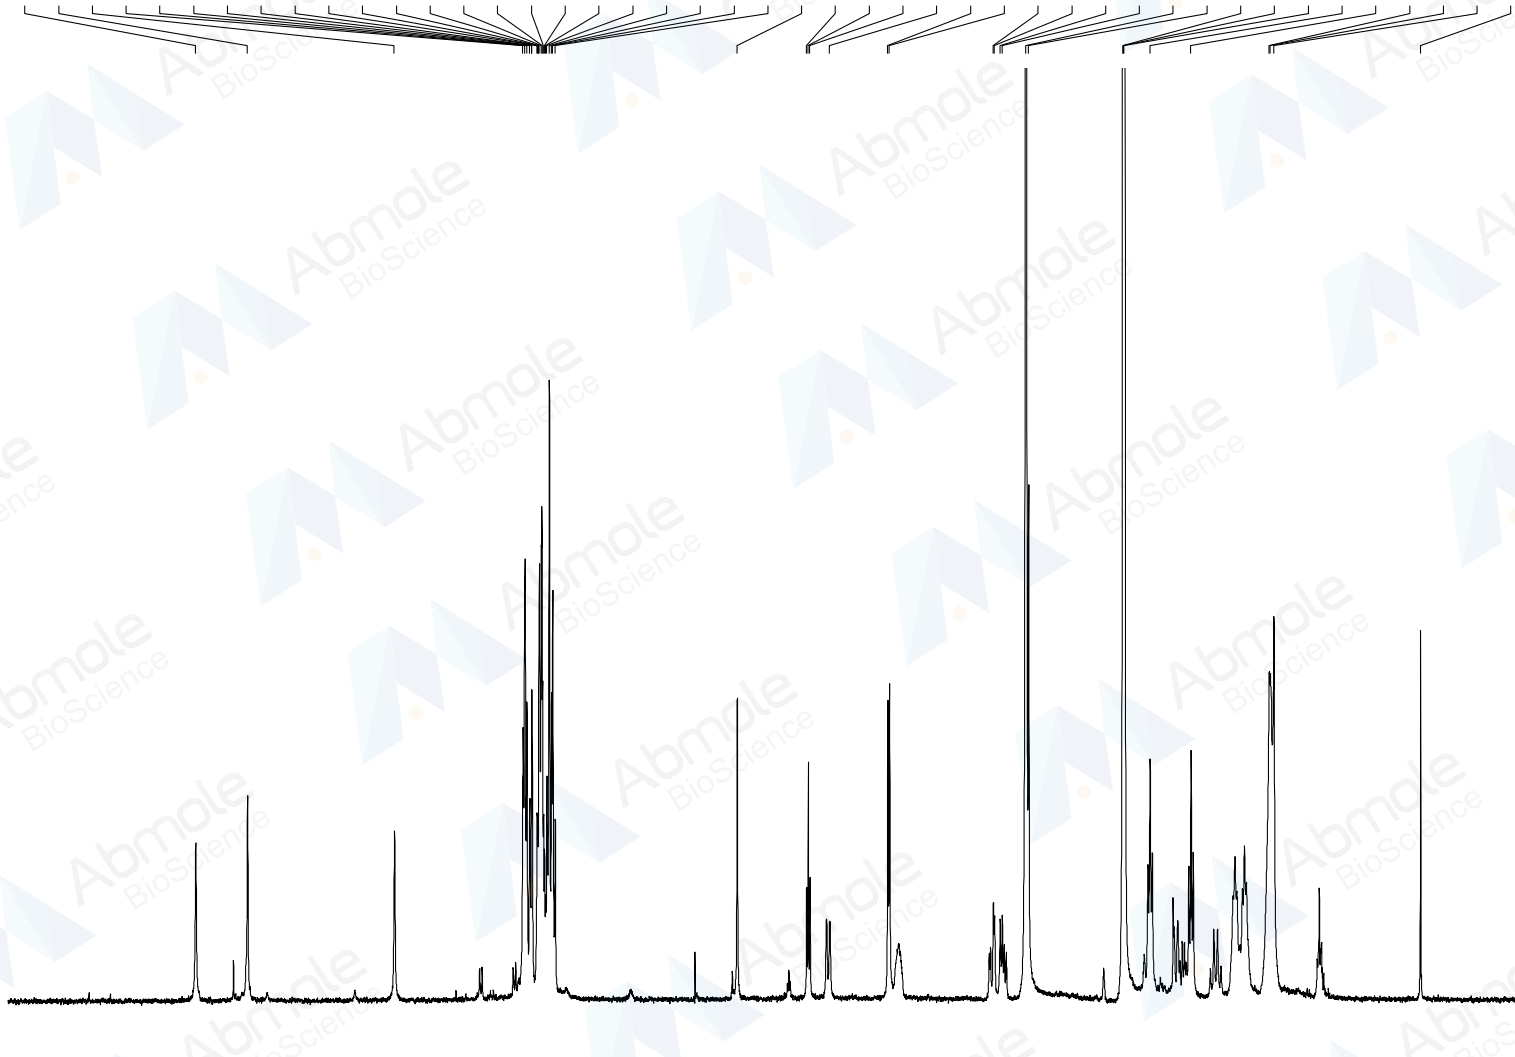

0.80  
0.99  
0.88  
15.30  
1.00  
1.02  
0.83  
2.54  
1.80  
21.83  
2.70  
3.35  
1.02  
4.03  
6.54  
0.94

Current Data Parameters  
NAME Tubacin 01  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20170601  
Time\_ 13.25  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8278.146 Hz  
FIDRES 0.126314 Hz  
AQ 3.9584243 sec  
RG 362  
DW 60.400 usec  
DE 8.00 usec  
TE 297.2 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
NUC1 1H  
P1 10.70 usec  
PL1 -3.00 dB  
SFO1 400.1324710 MHz

F2 - Processing parameters  
SI 32768  
SF 400.130000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00