

8.101
8.098
7.715
7.712
7.709
7.698
7.694
7.689
7.678
7.675
7.672
7.566
7.562
7.547
7.532
7.527
7.284

— 1.586

— 0.025




Current Data Parameters
NAME Benzoyl Peroxide-01
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170731
Time_ 14.30
INSTRUM spect
PROBHD 5 mm PADUL 13C
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 8
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 199.46
DW 62.400 usec
DE 6.50 usec
TE 297.8 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 400.1324710 MHz
NUC1 1H
P1 10.00 usec
PLW1 20.00000000 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

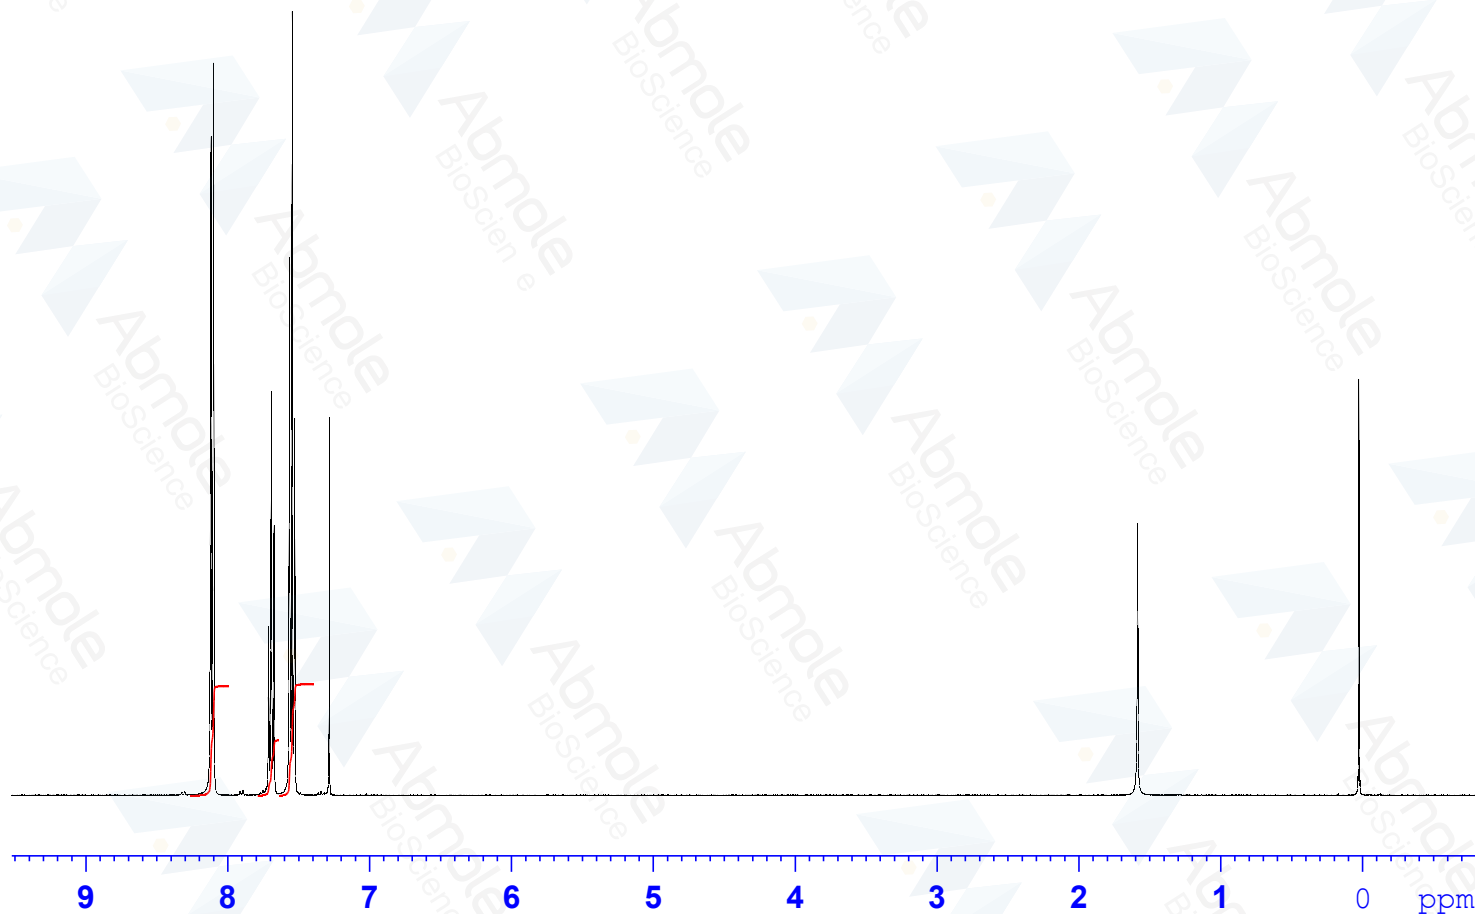

2.00
1.01
2.03