


=====

Acq. Operator	: System	Seq. Line	: 3
Acq. Instrument	: LC1260	Location	: Vial 69
Injection Date	: 7/20/2016 5:57:14 PM	Inj	: 1
		Inj Volume	: 0 µl
Different Inj Volume from Sequence !		Actual Inj Volume	: 6 µl
Acq. Method	: E:\DATA\20160719\20130913-01 2016-07-20 17-04-58\10-80AD 15MIN.M		
Last changed	: 7/20/2016 5:04:58 PM by System		
Analysis Method	: D:\PUBLIC\20160719\DEF_LC 2016-07-19 17-29-35\YH-20160719-2.D\DA.M (5-95 6MIN.M)		
Last changed	: 7/21/2016 9:11:59 AM		
	(modified after loading)		

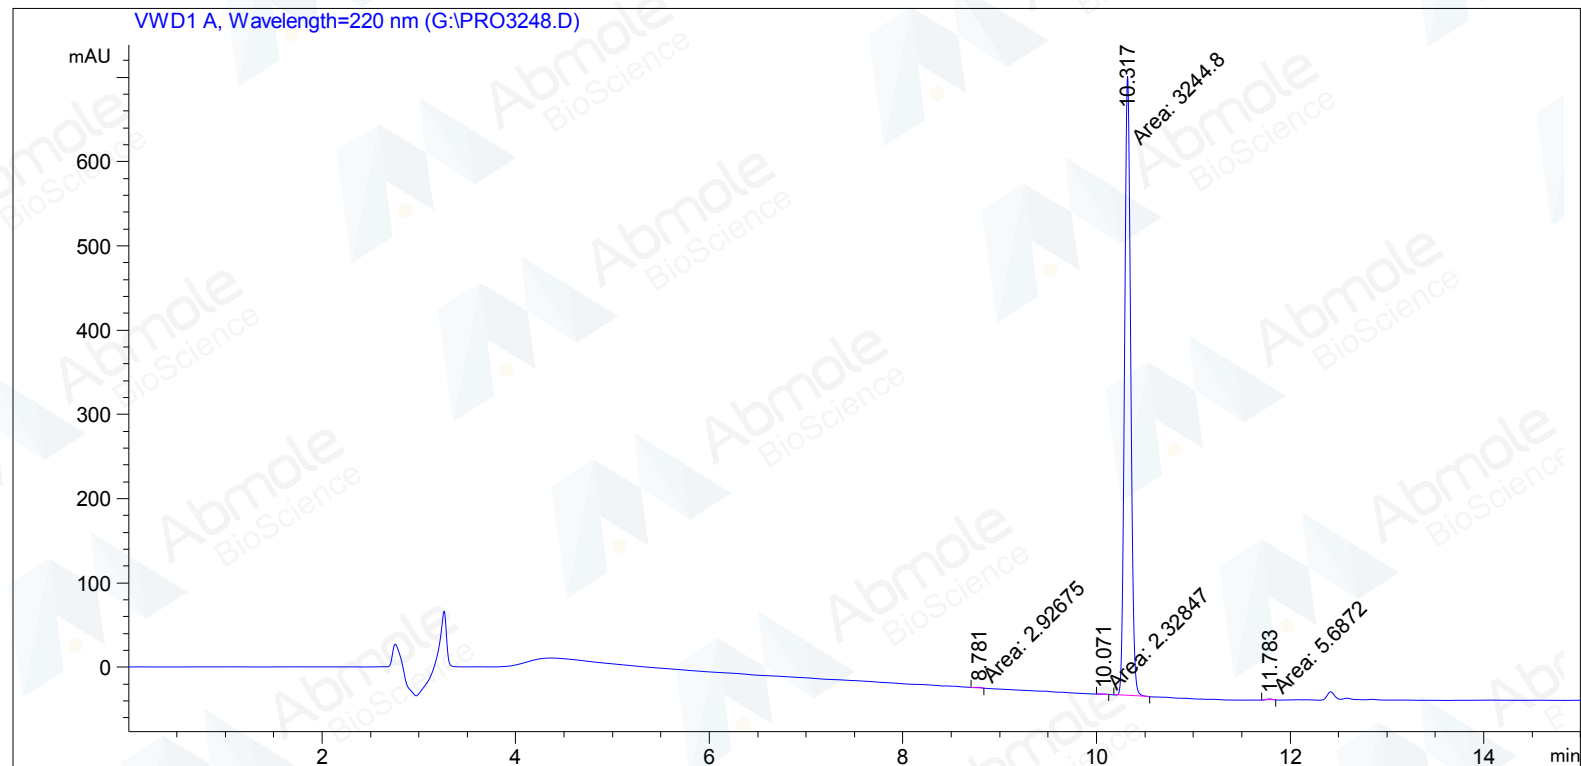

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=220 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.781	MM	0.0716	2.92675	6.81545e-1	0.0899
2	10.071	MM	0.0833	2.32847	4.66091e-1	0.0715

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
3	10.317	MM	0.0735	3244.80225	735.70801	99.6639
4	11.783	MM	0.0749	5.68720	1.26470	0.1747

Totals : 3255.74467 738.12034

*** End of Report ***